

FIG. 1 PRIOR ART

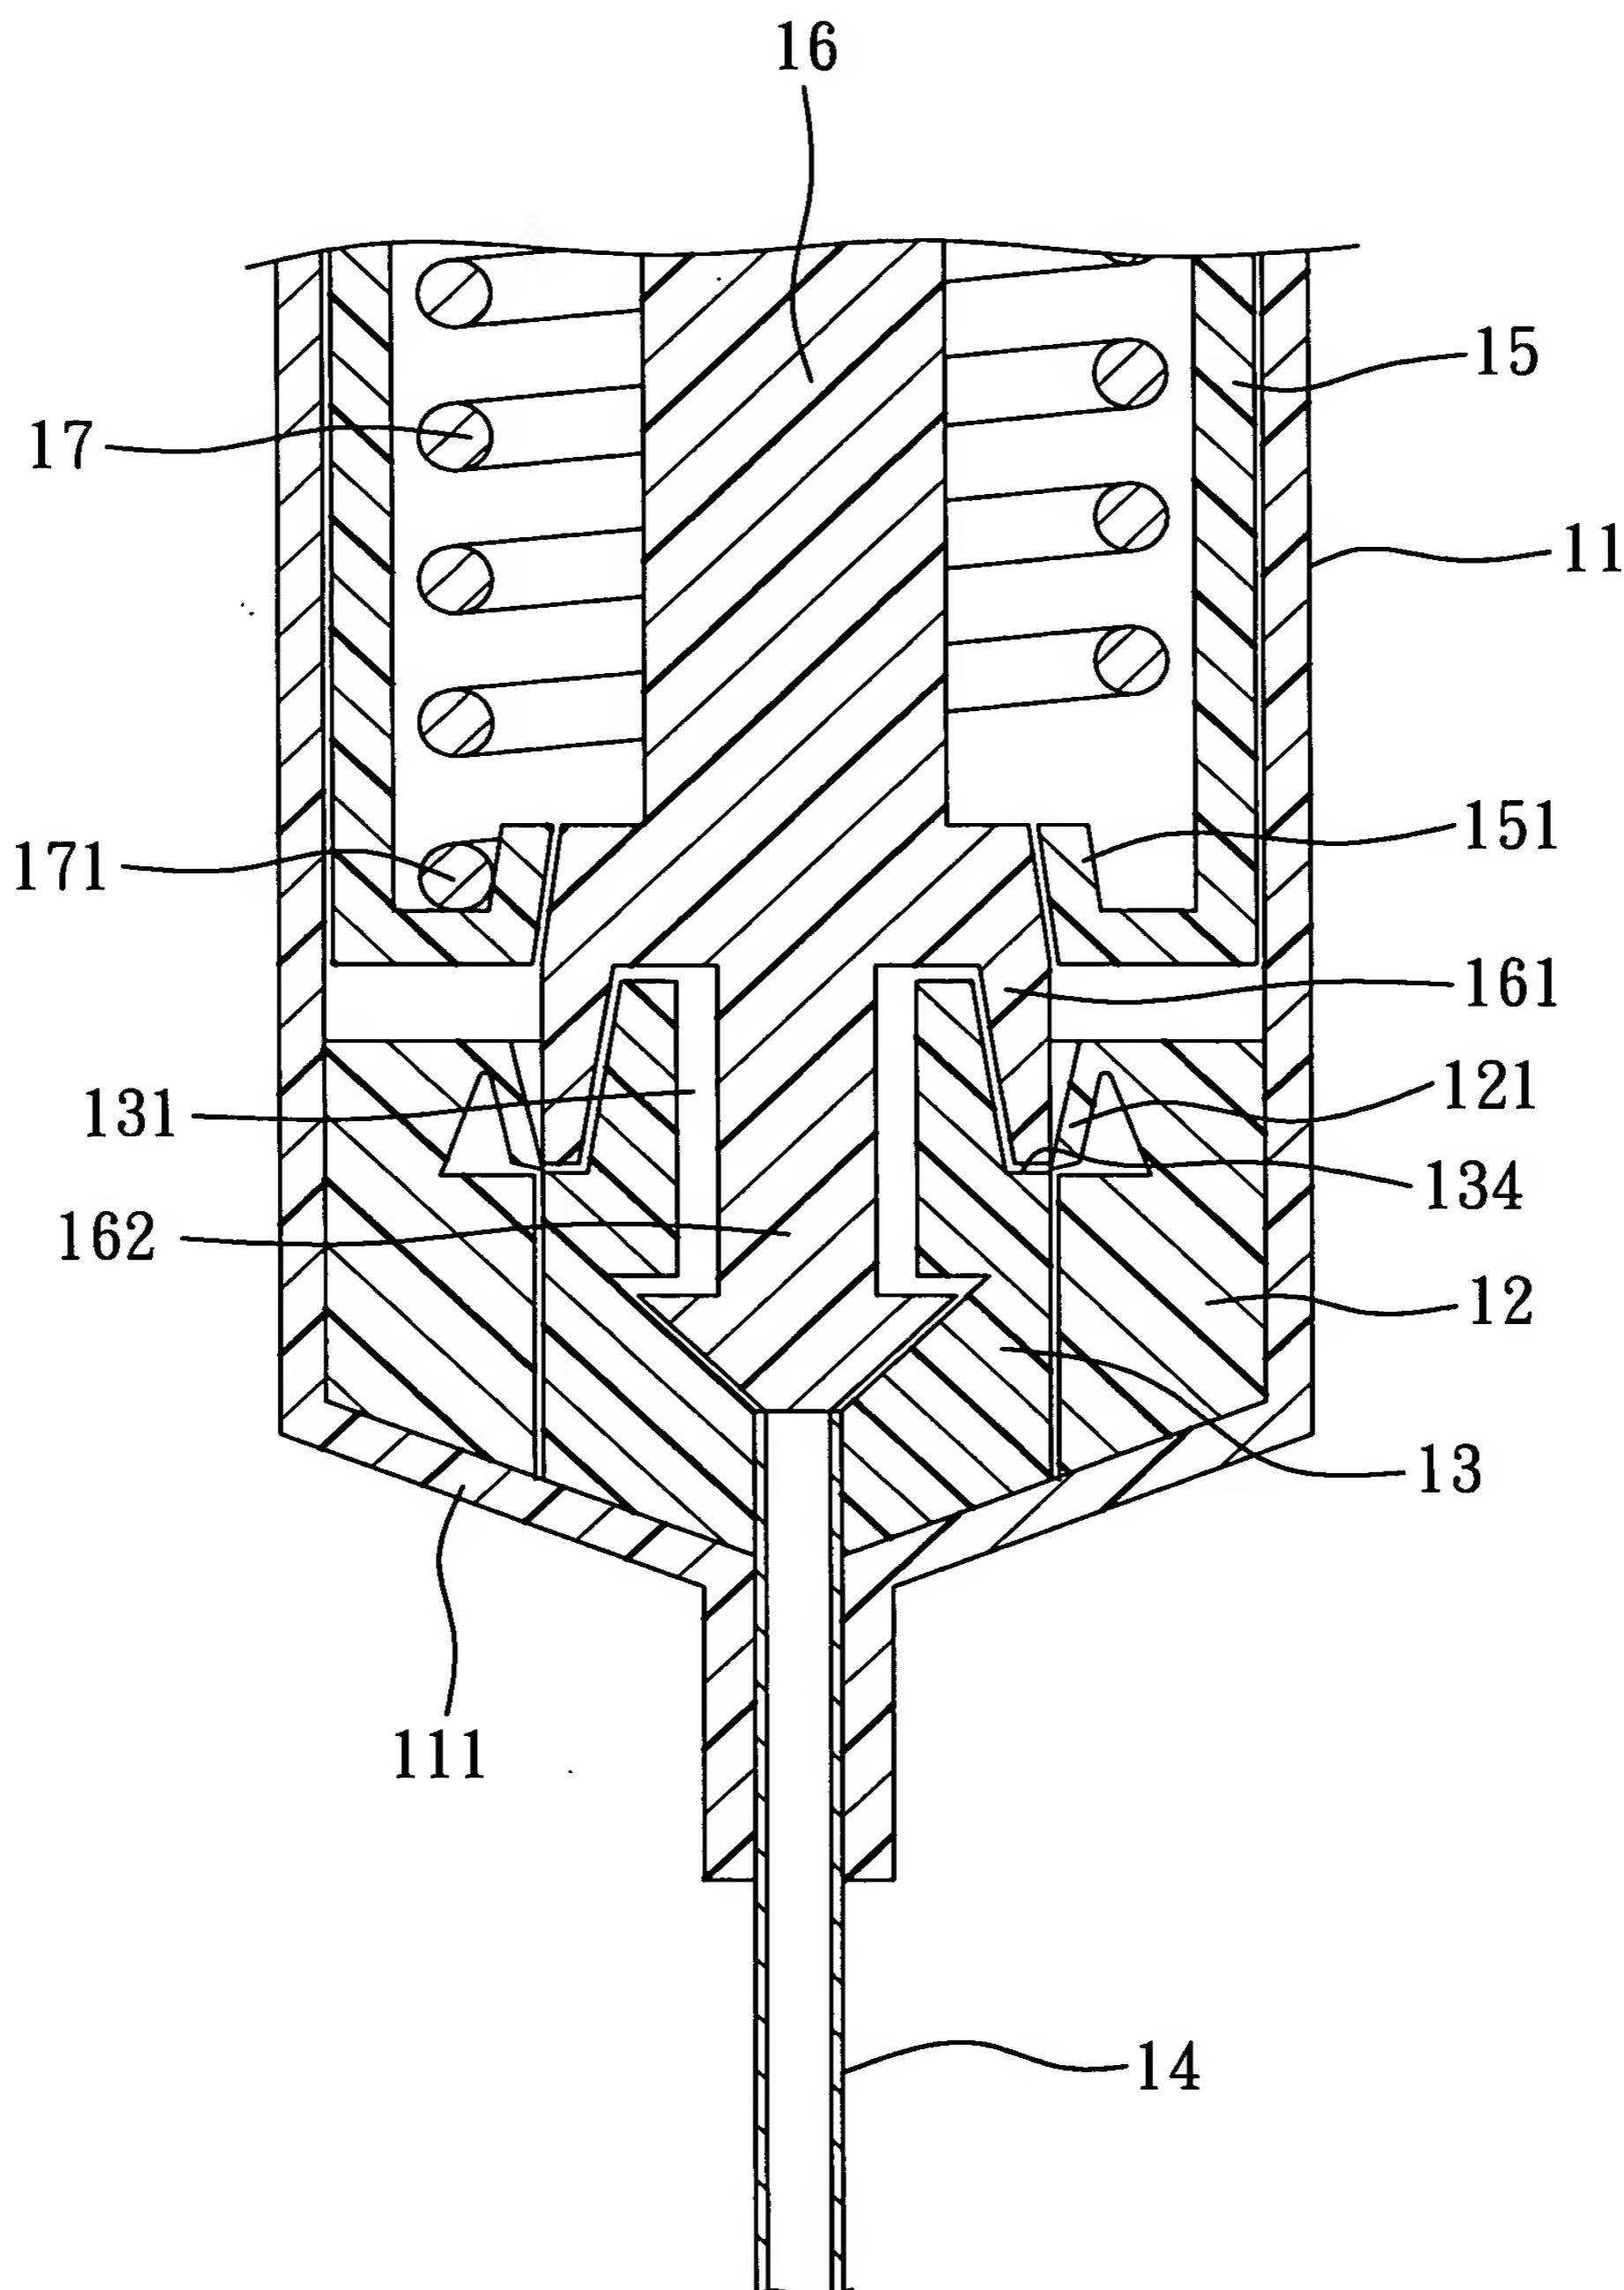


FIG. 2
PRIOR ART

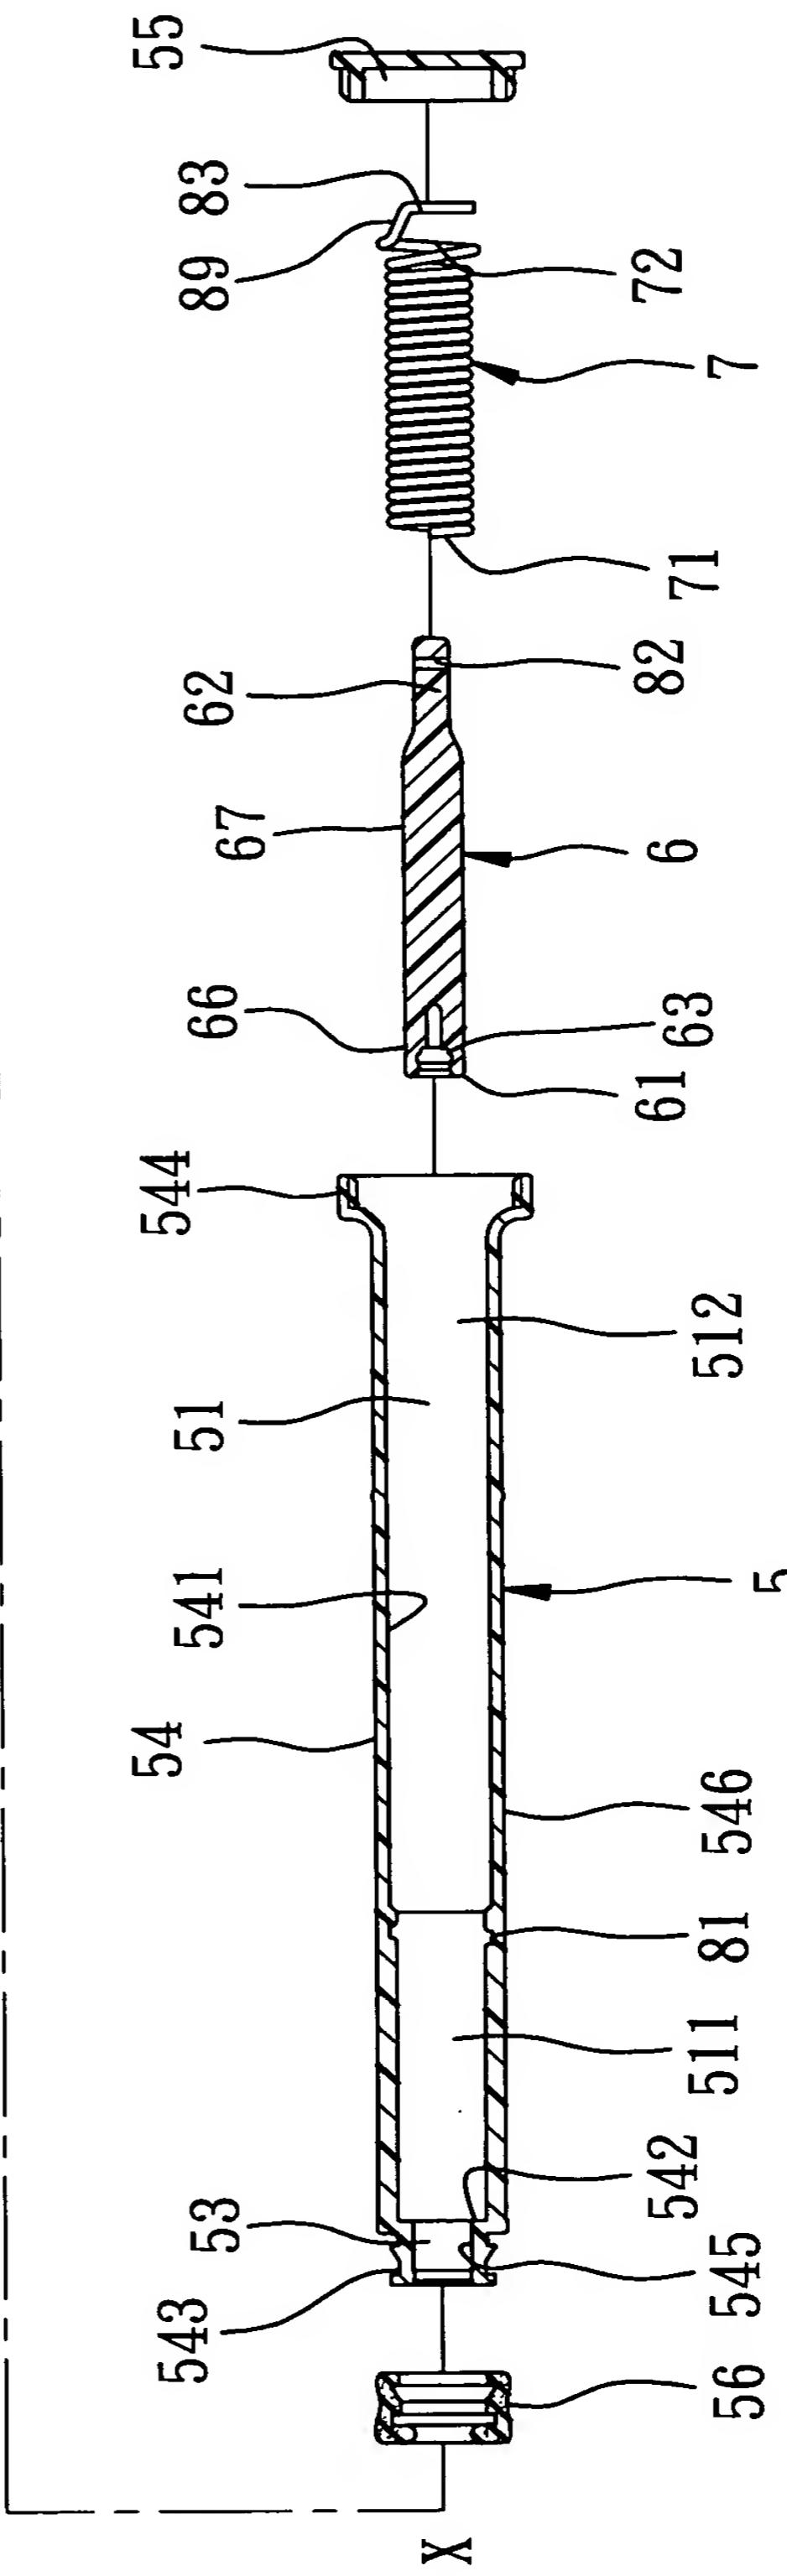
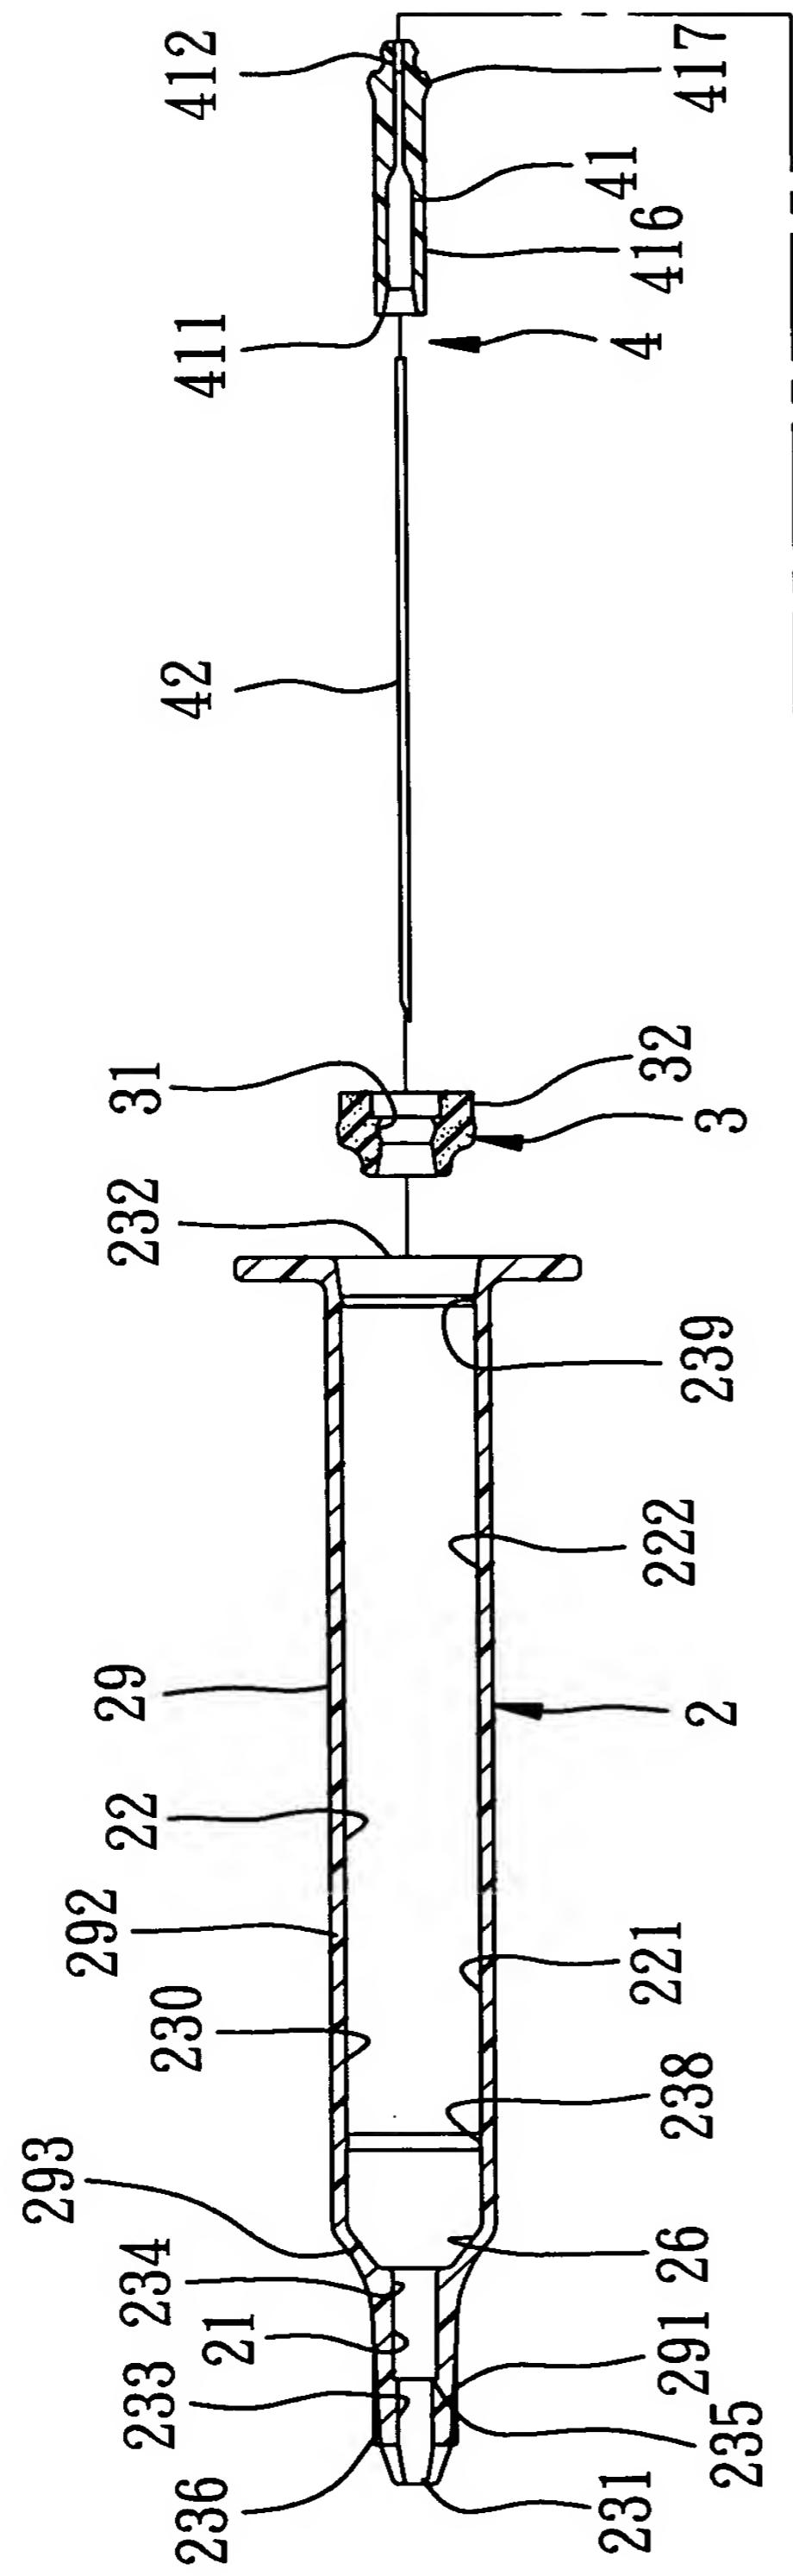


FIG. 3

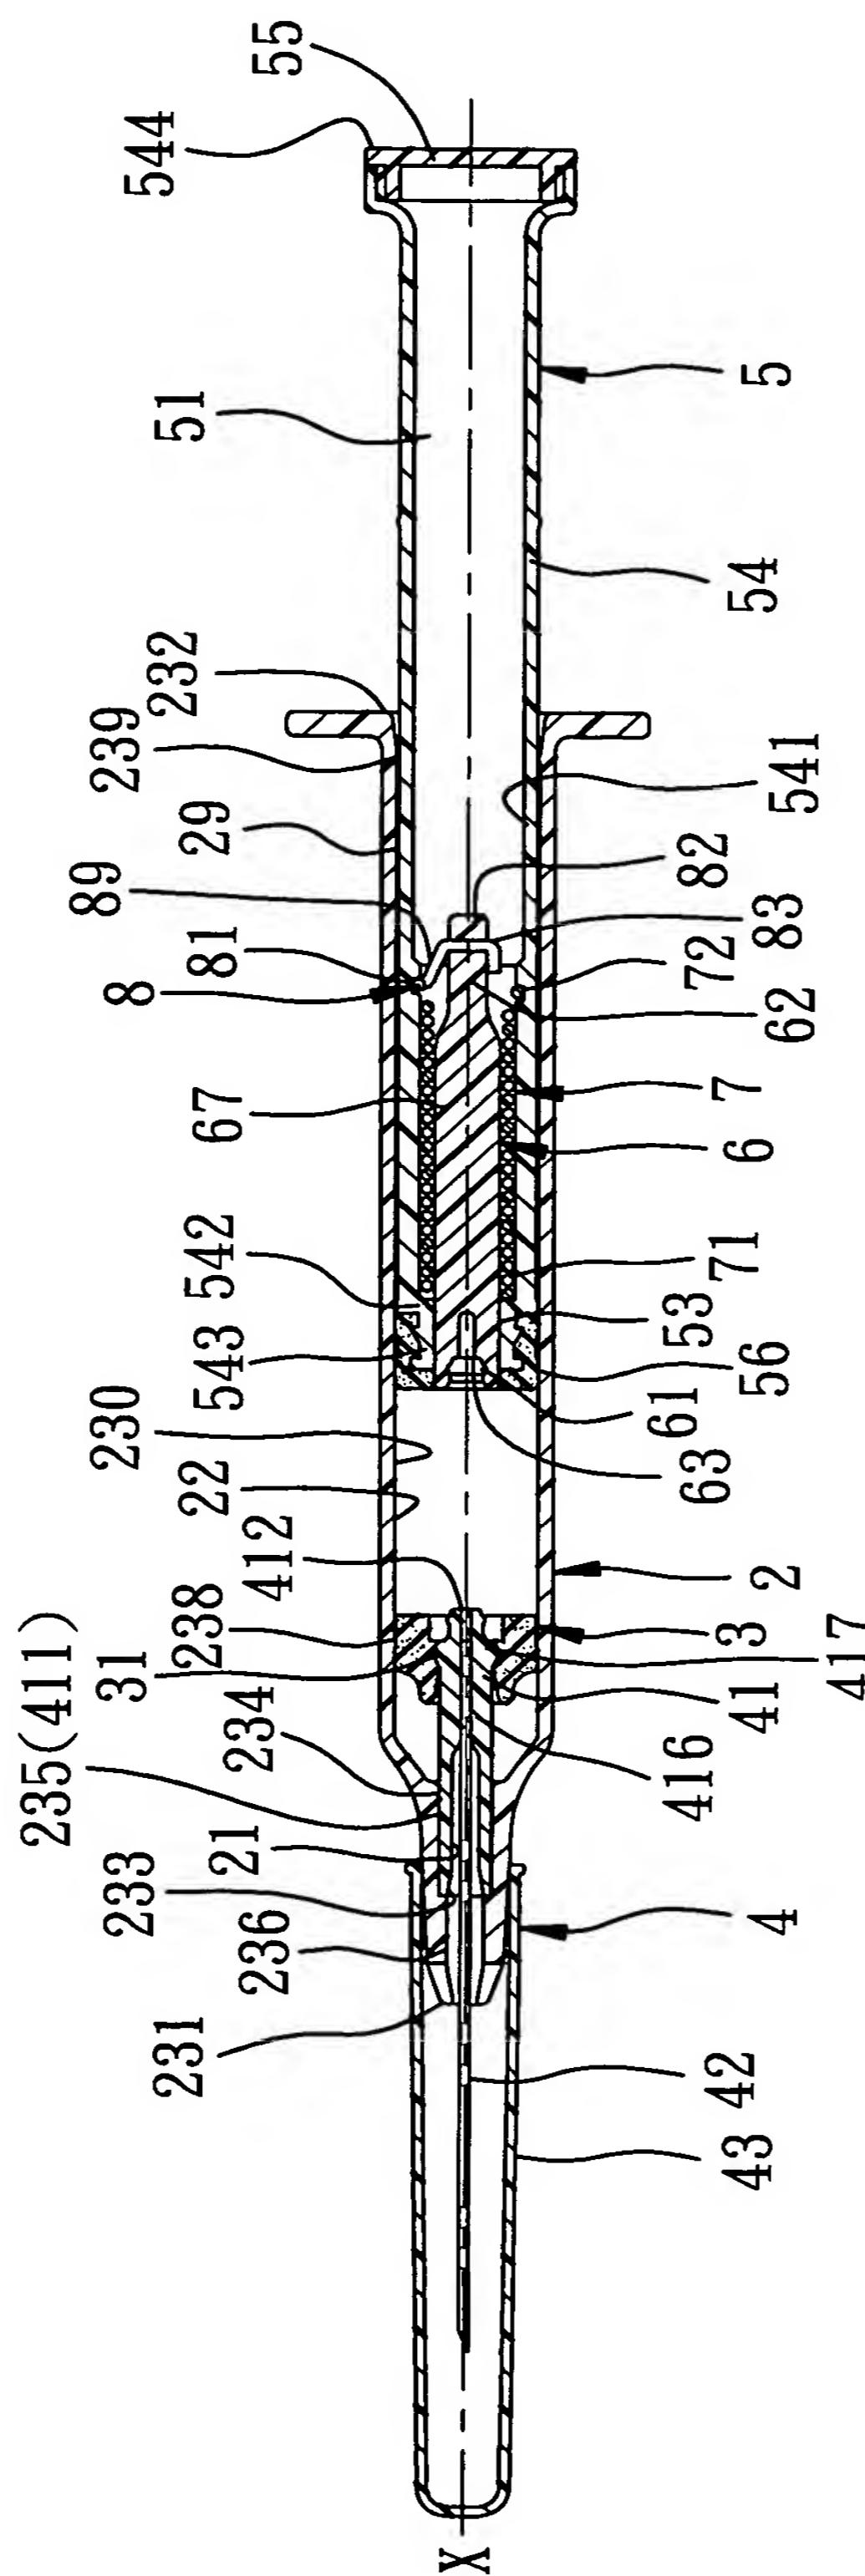


FIG. 4

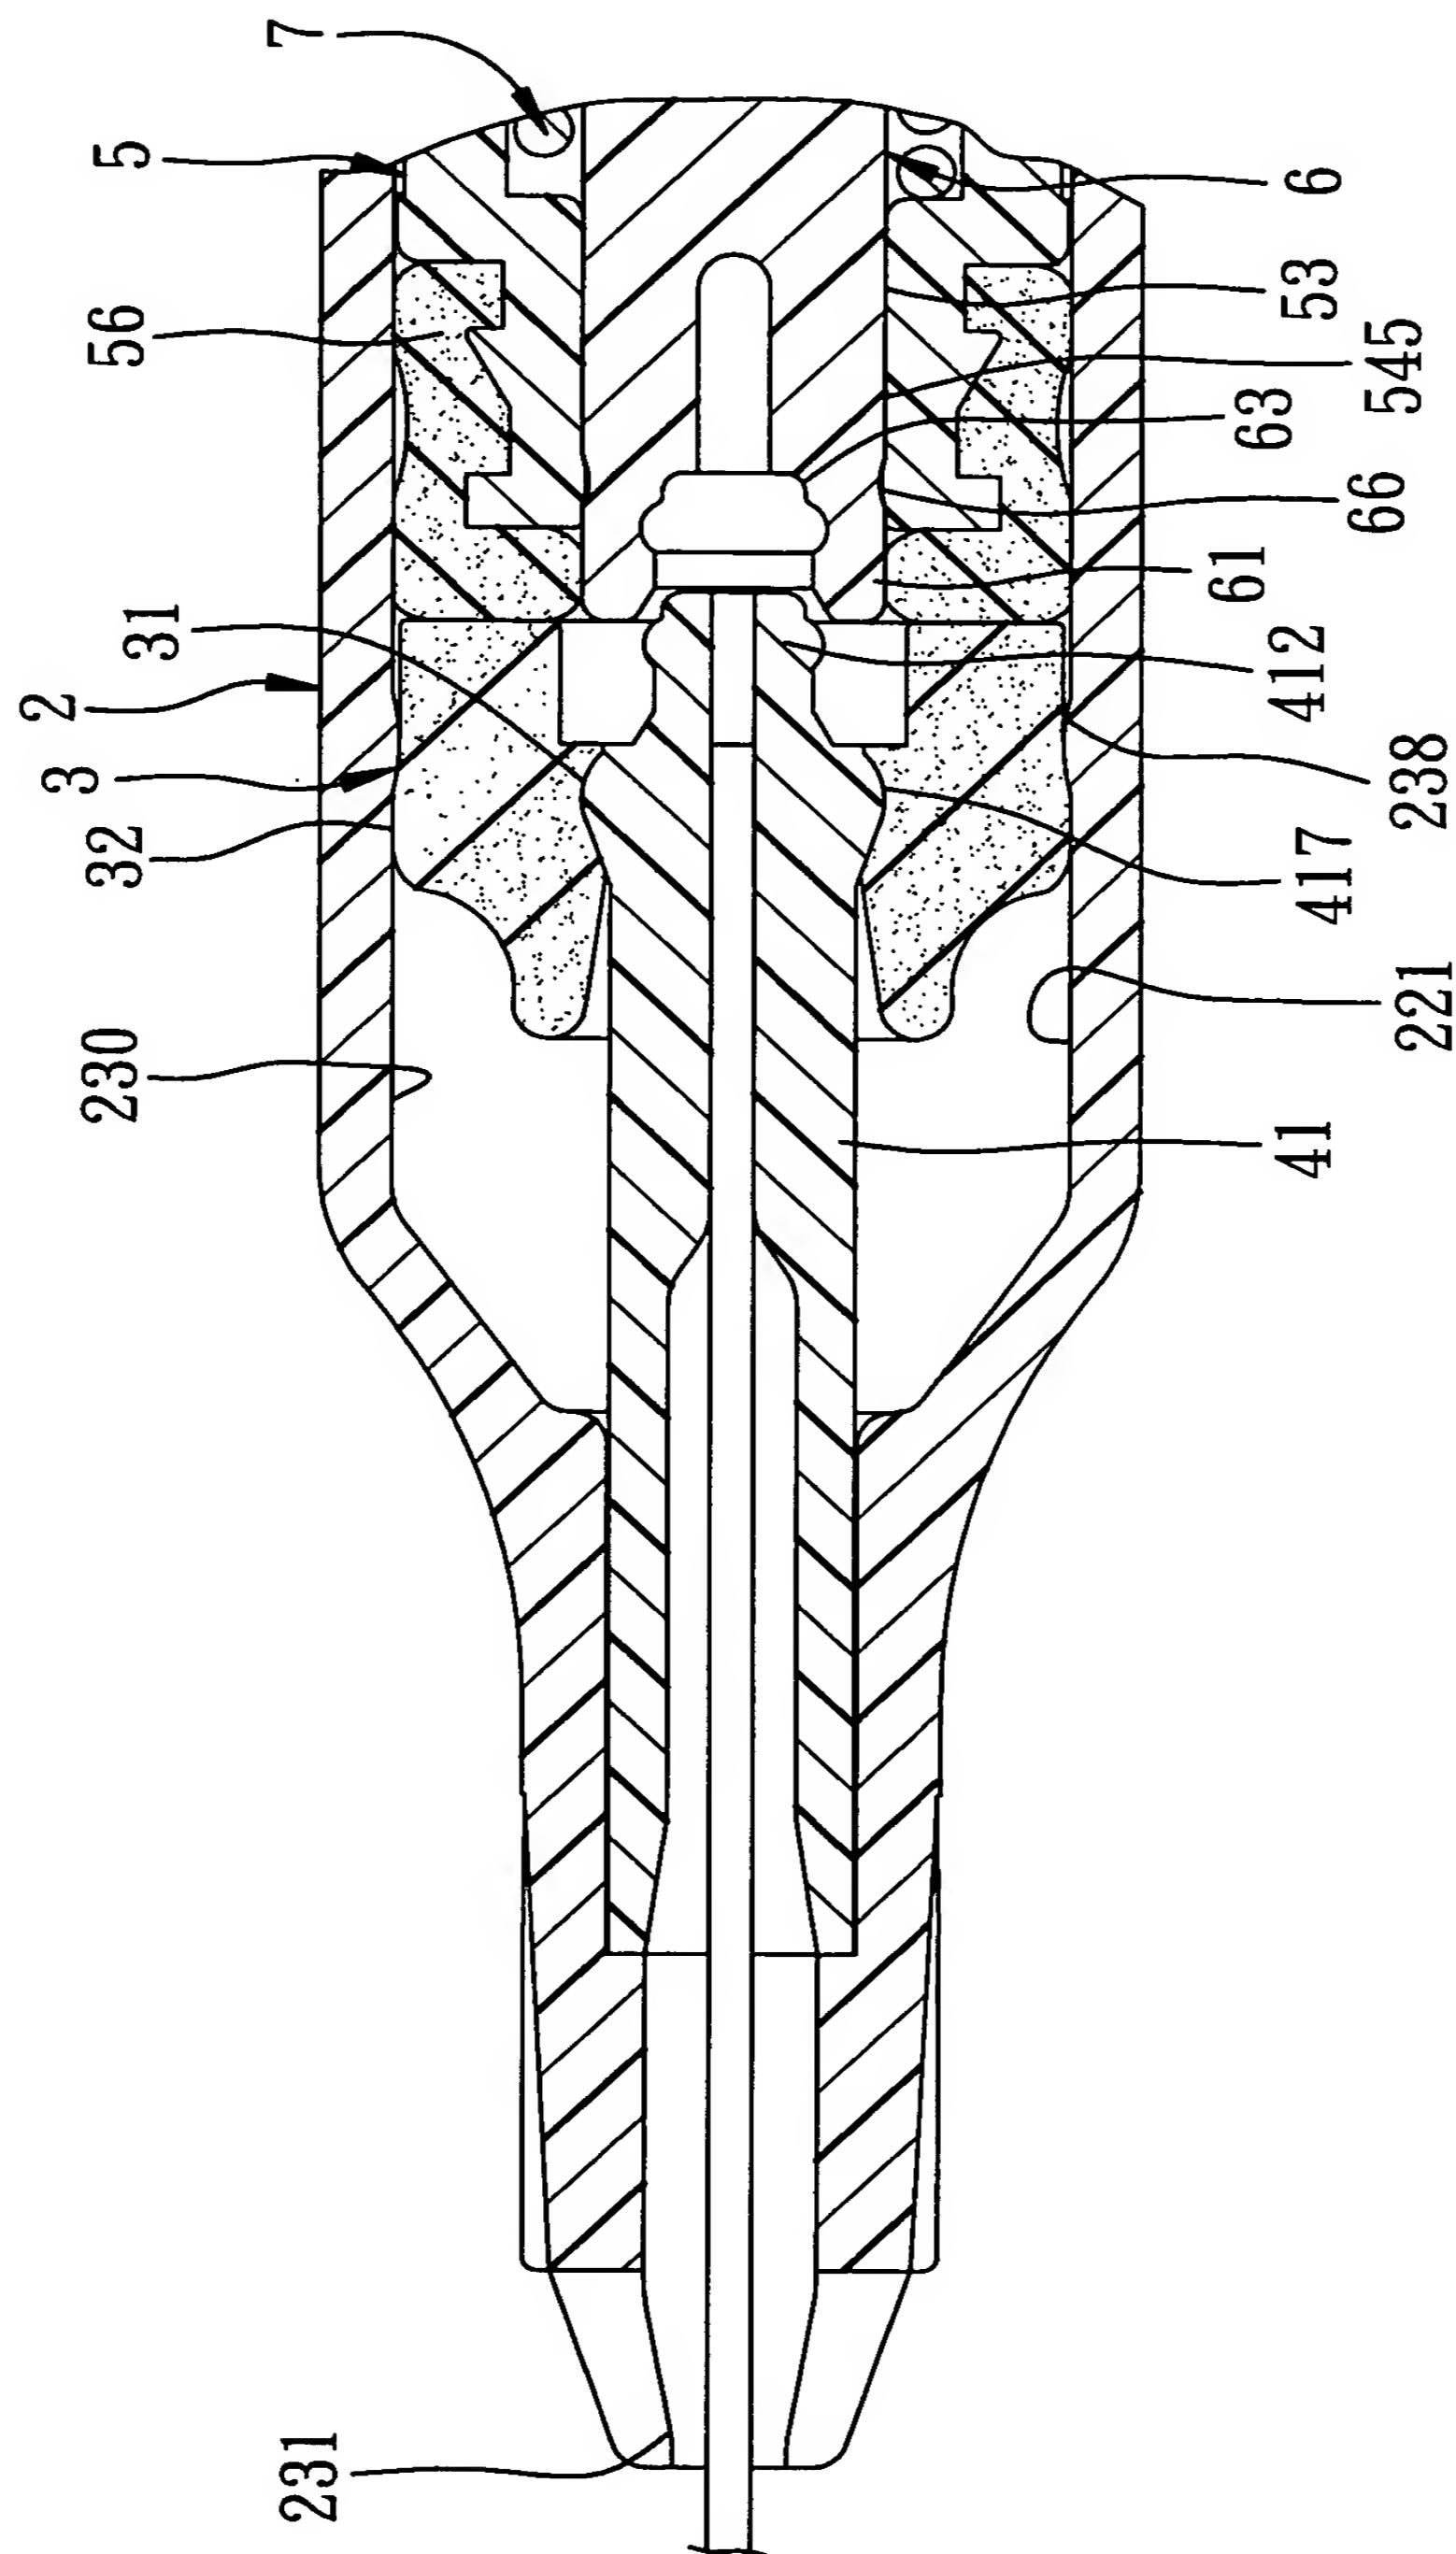


FIG. 5

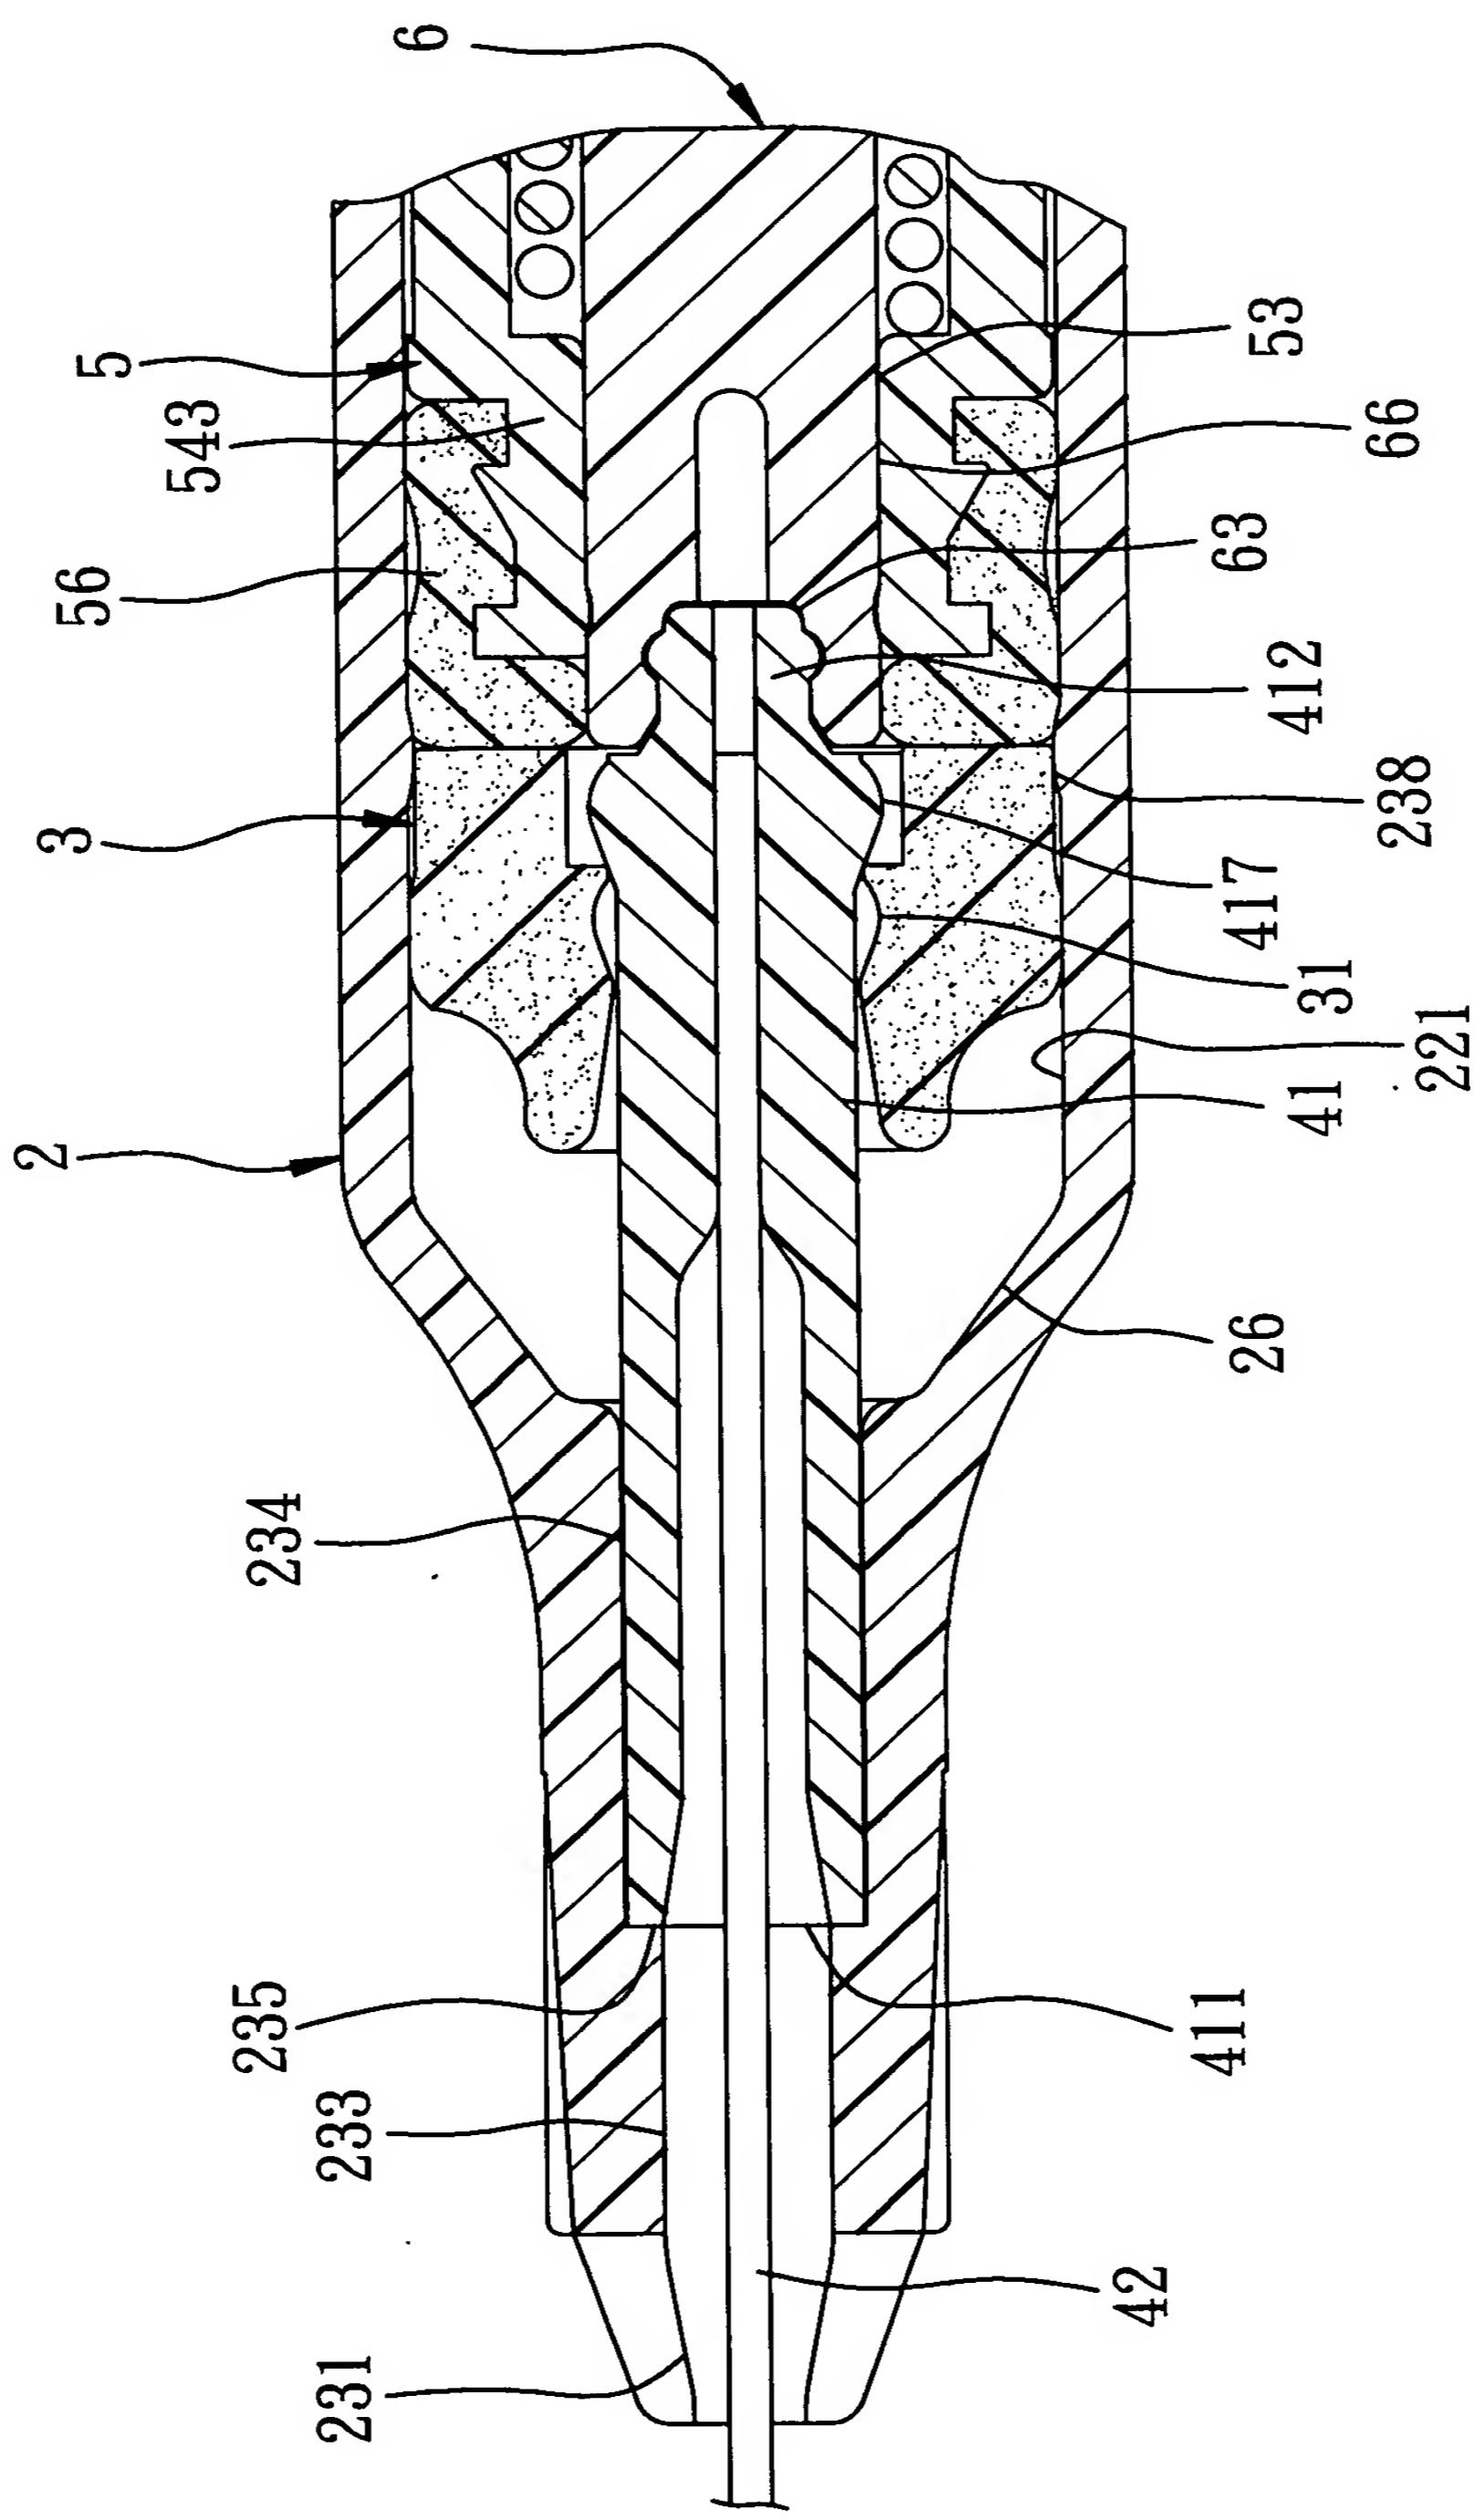


FIG. 6

DISPOSABLE SYRINGE

Shue et al.

Filed Sept. 22, 2003

Docket #48006-4

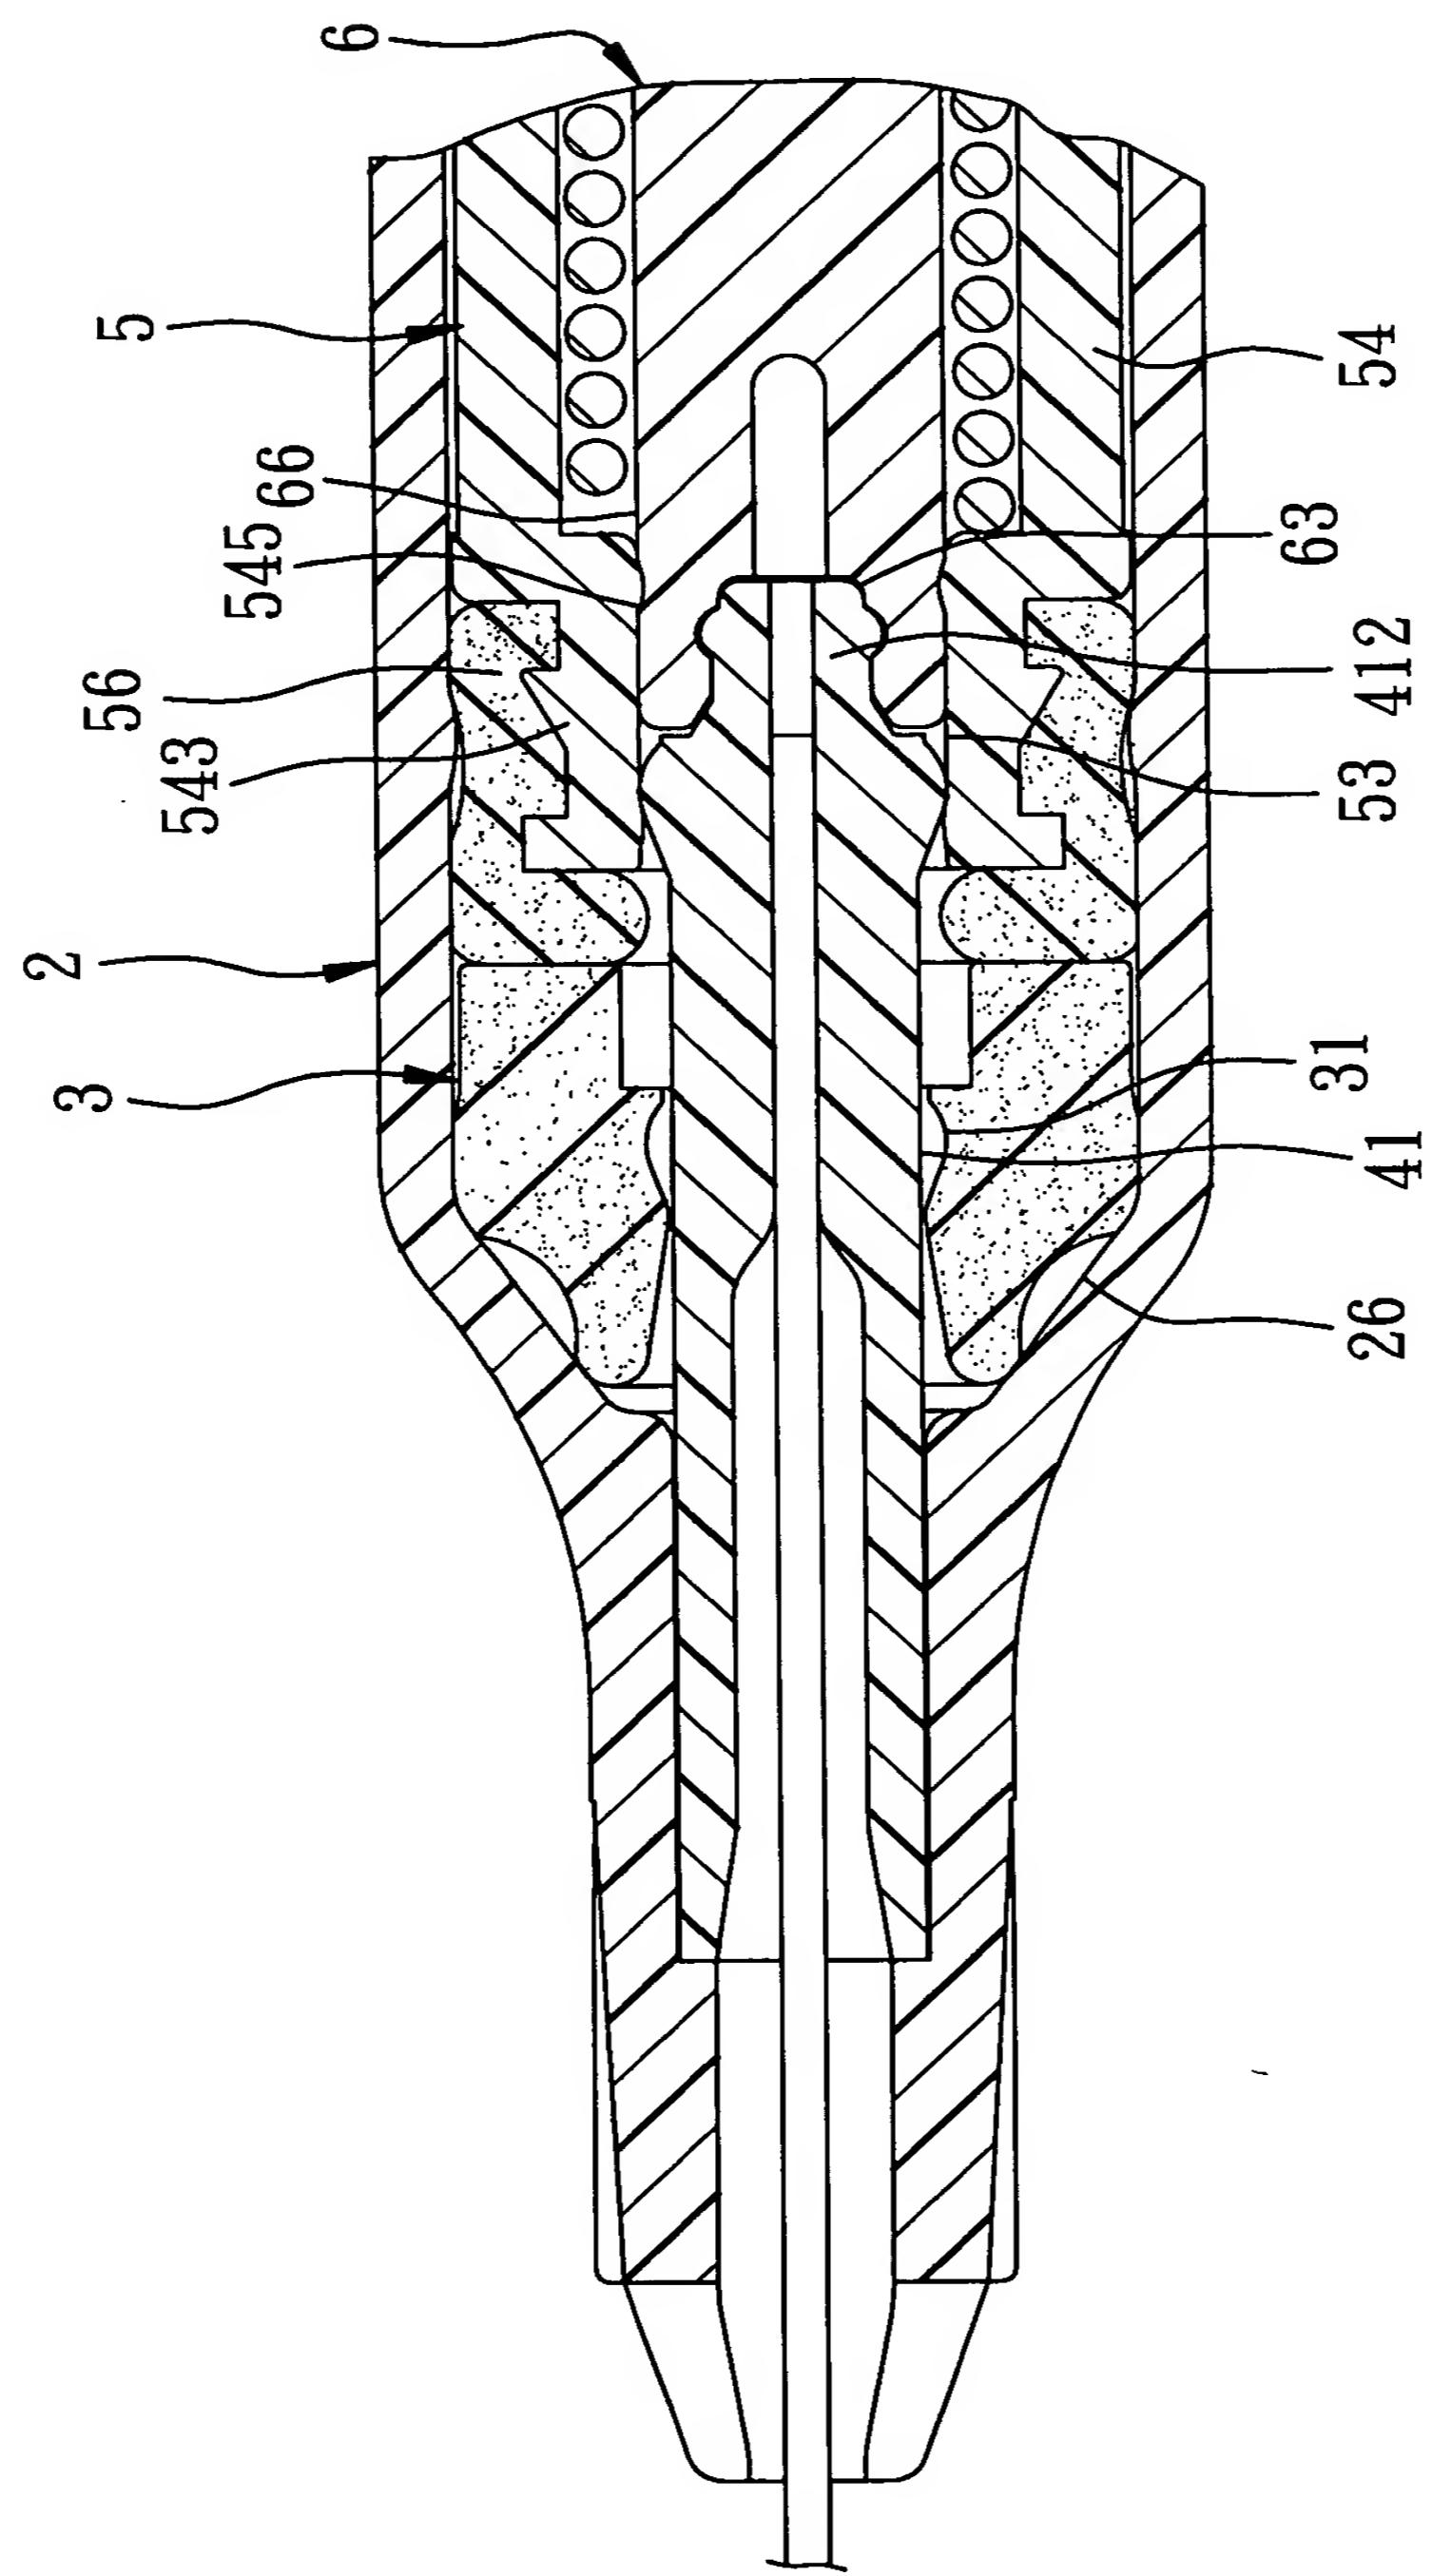


FIG. 7

DISPOSABLE SYRINGE

Shue et al.

Filed Sept. 22, 2003

Docket #48006-4

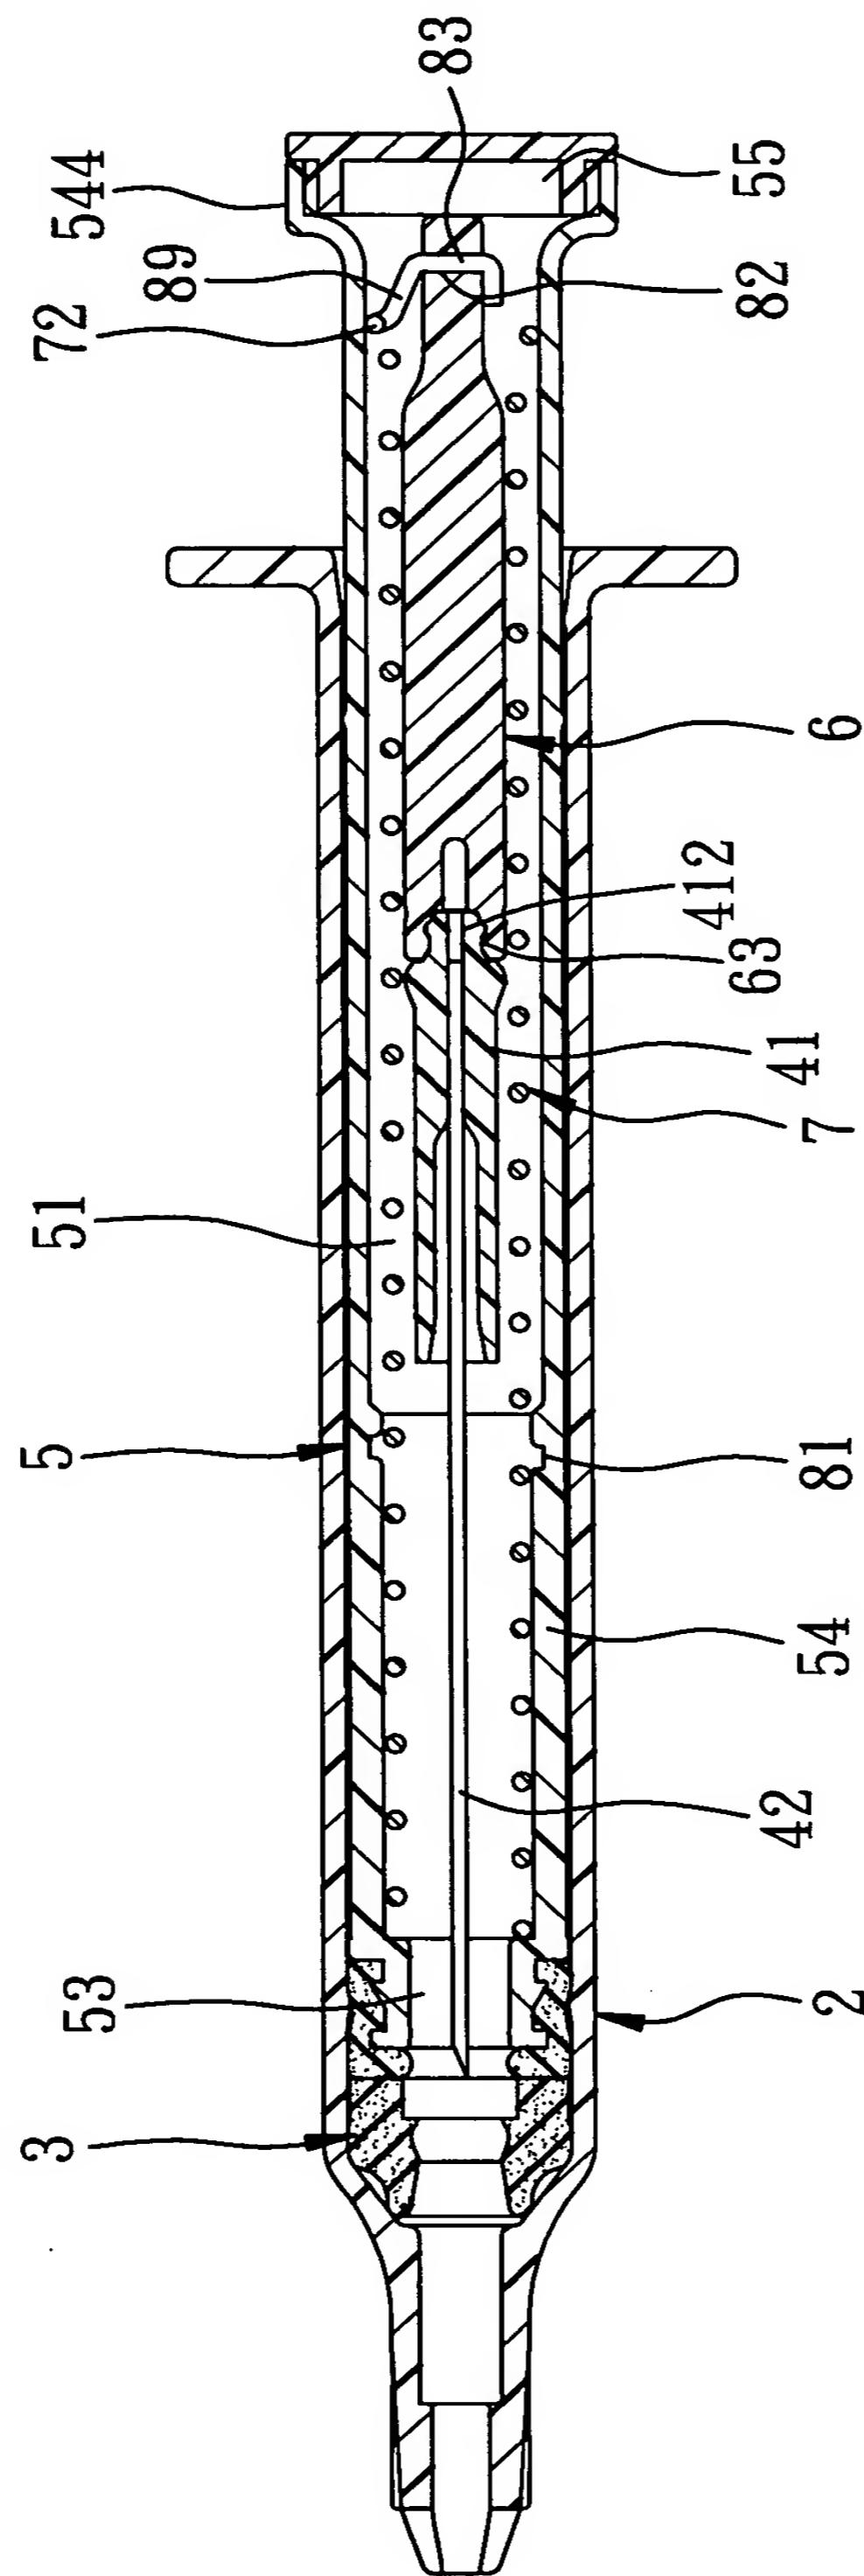


FIG. 8

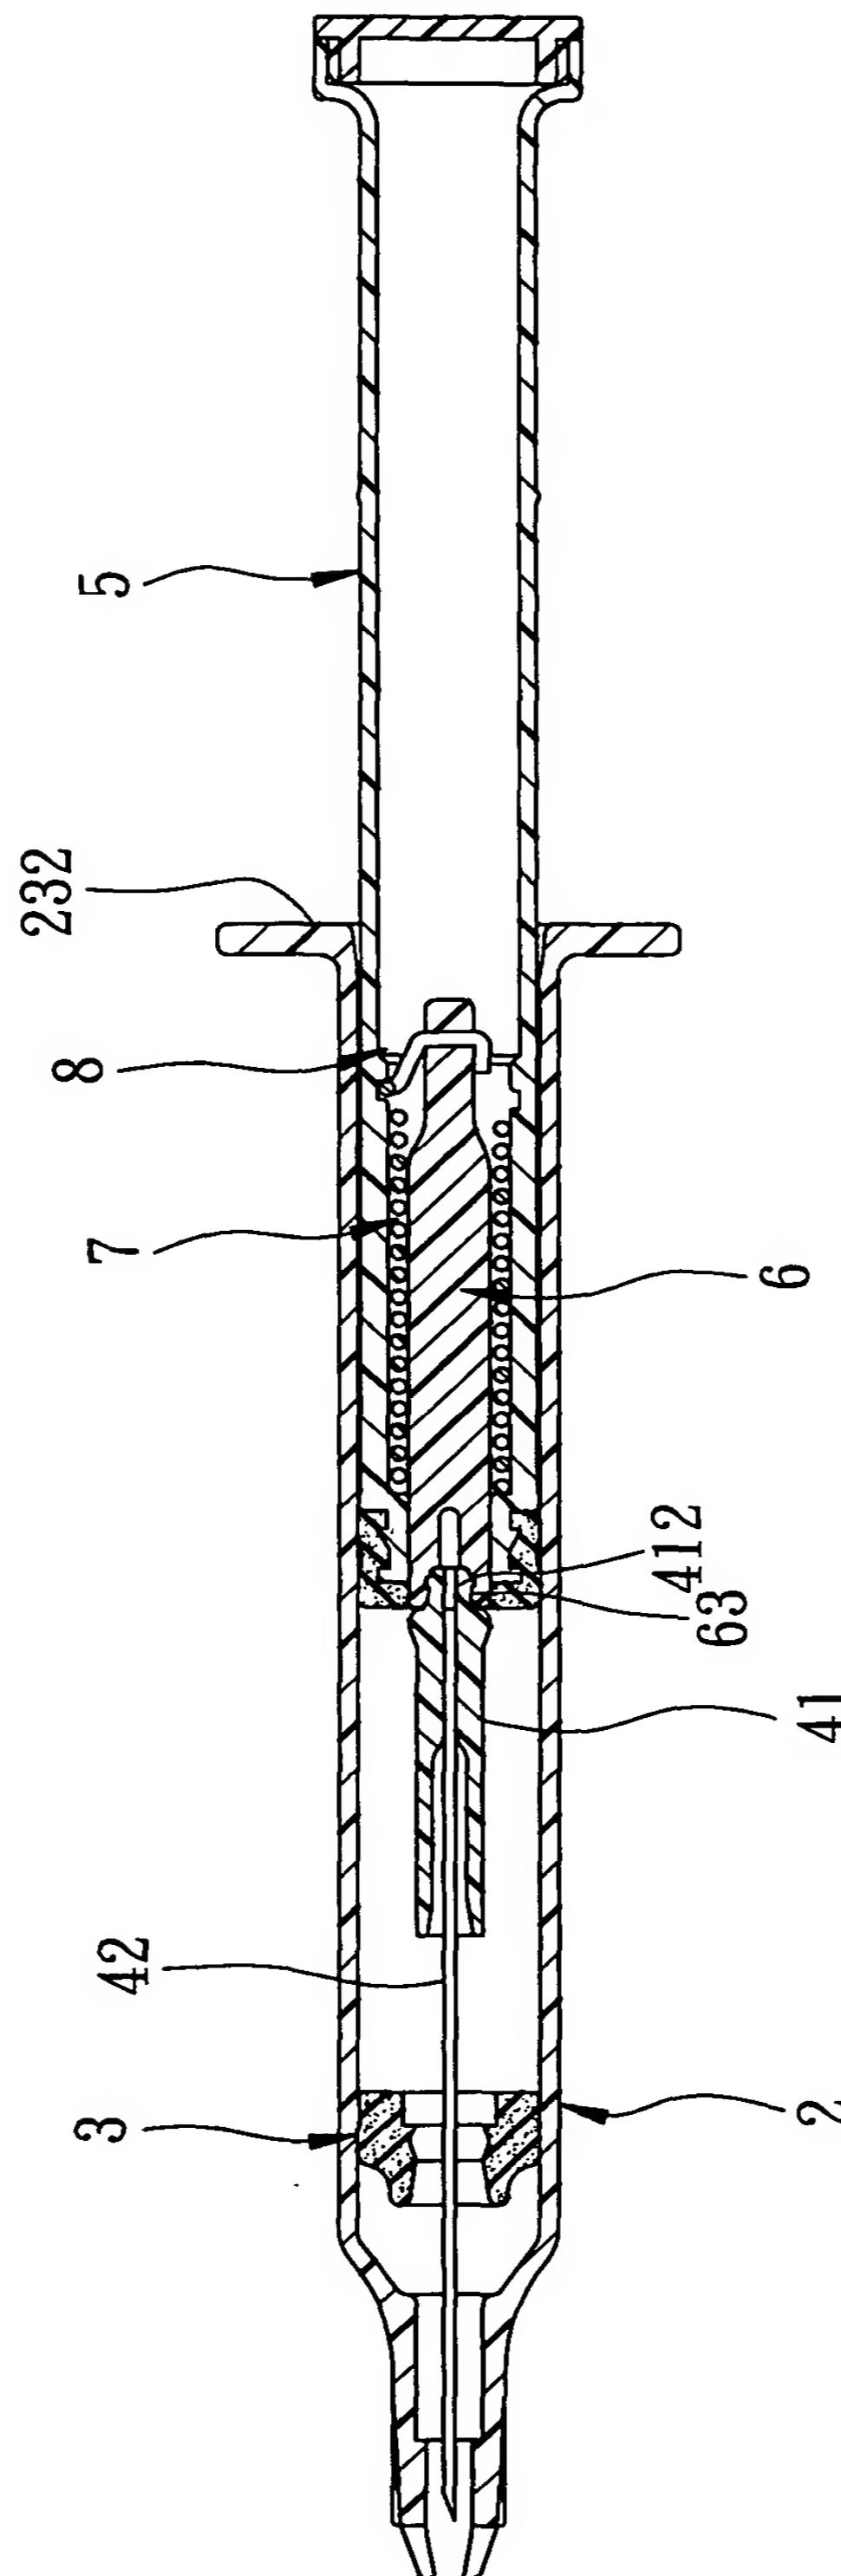


FIG. 9

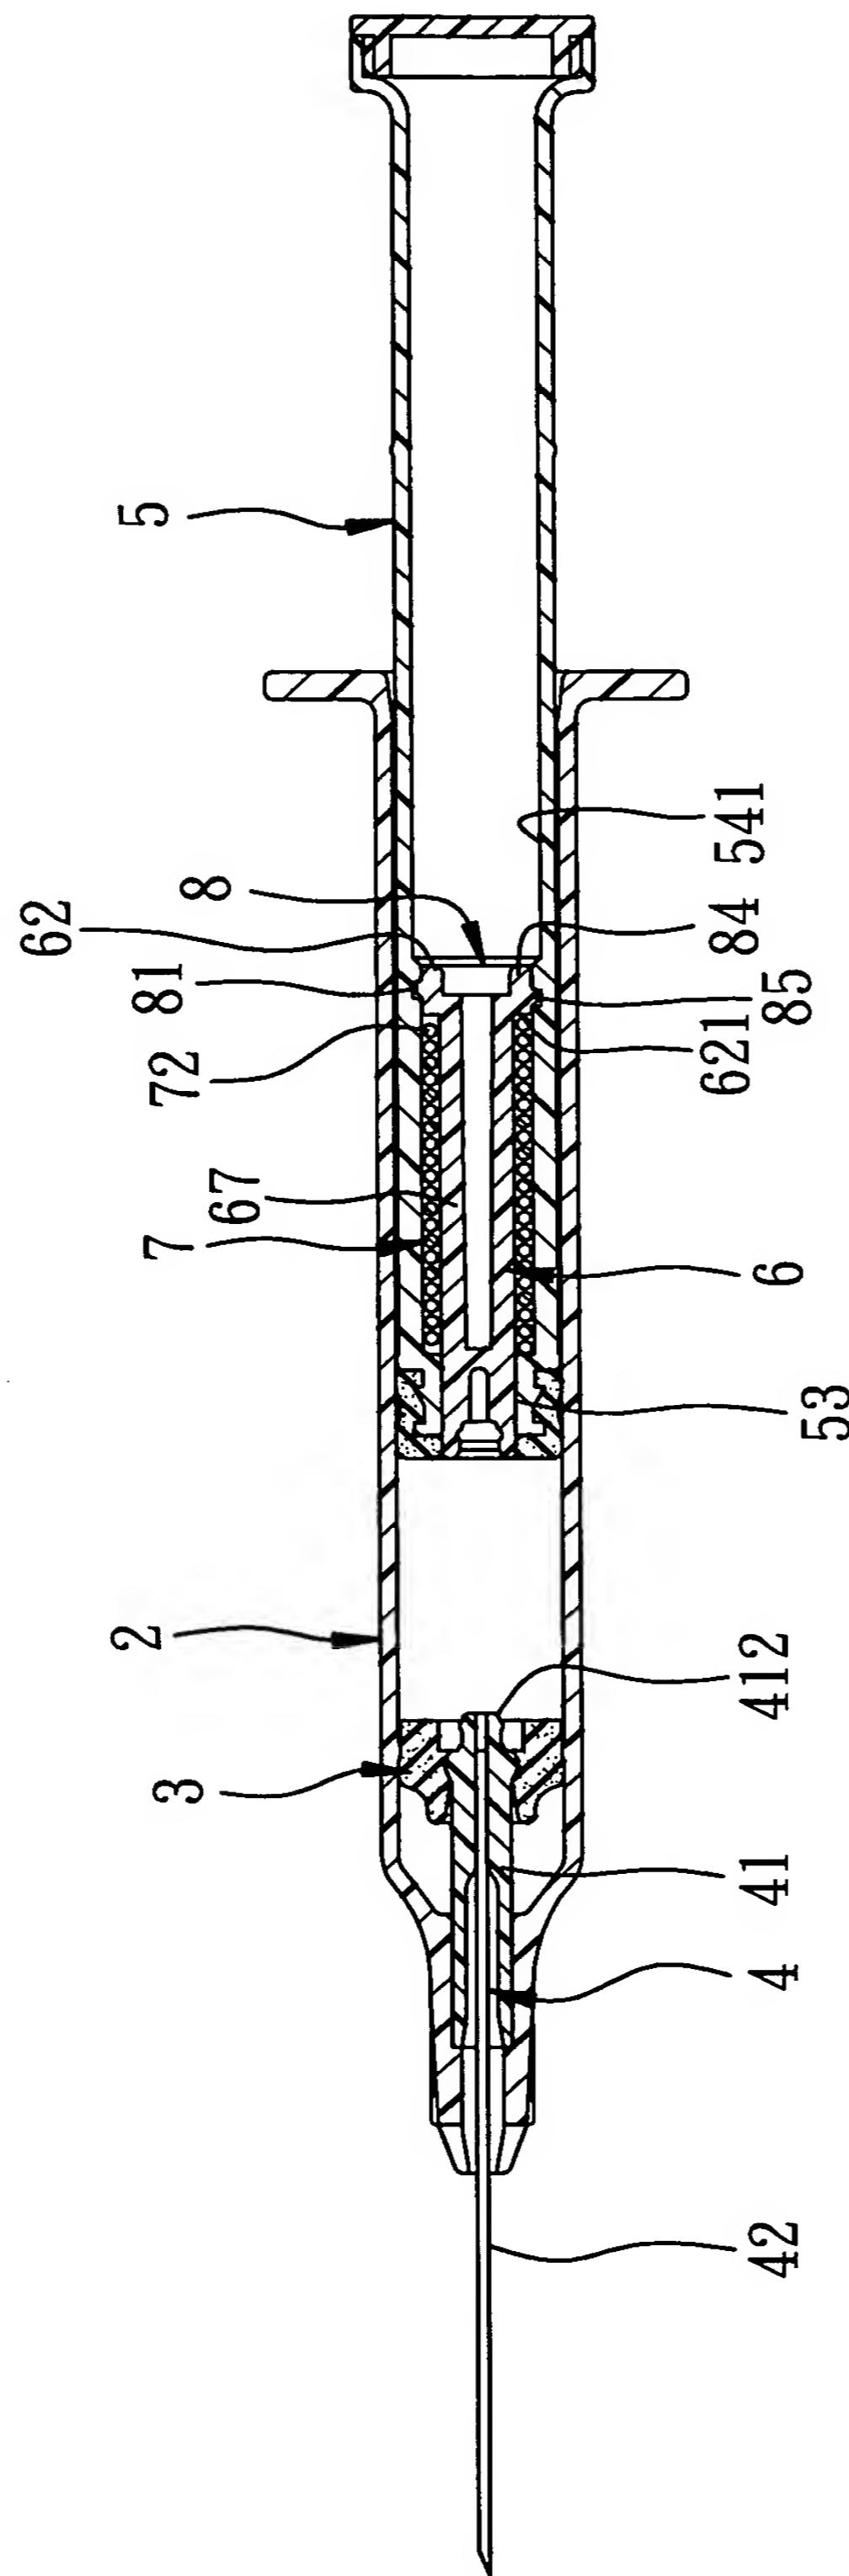


FIG. 10

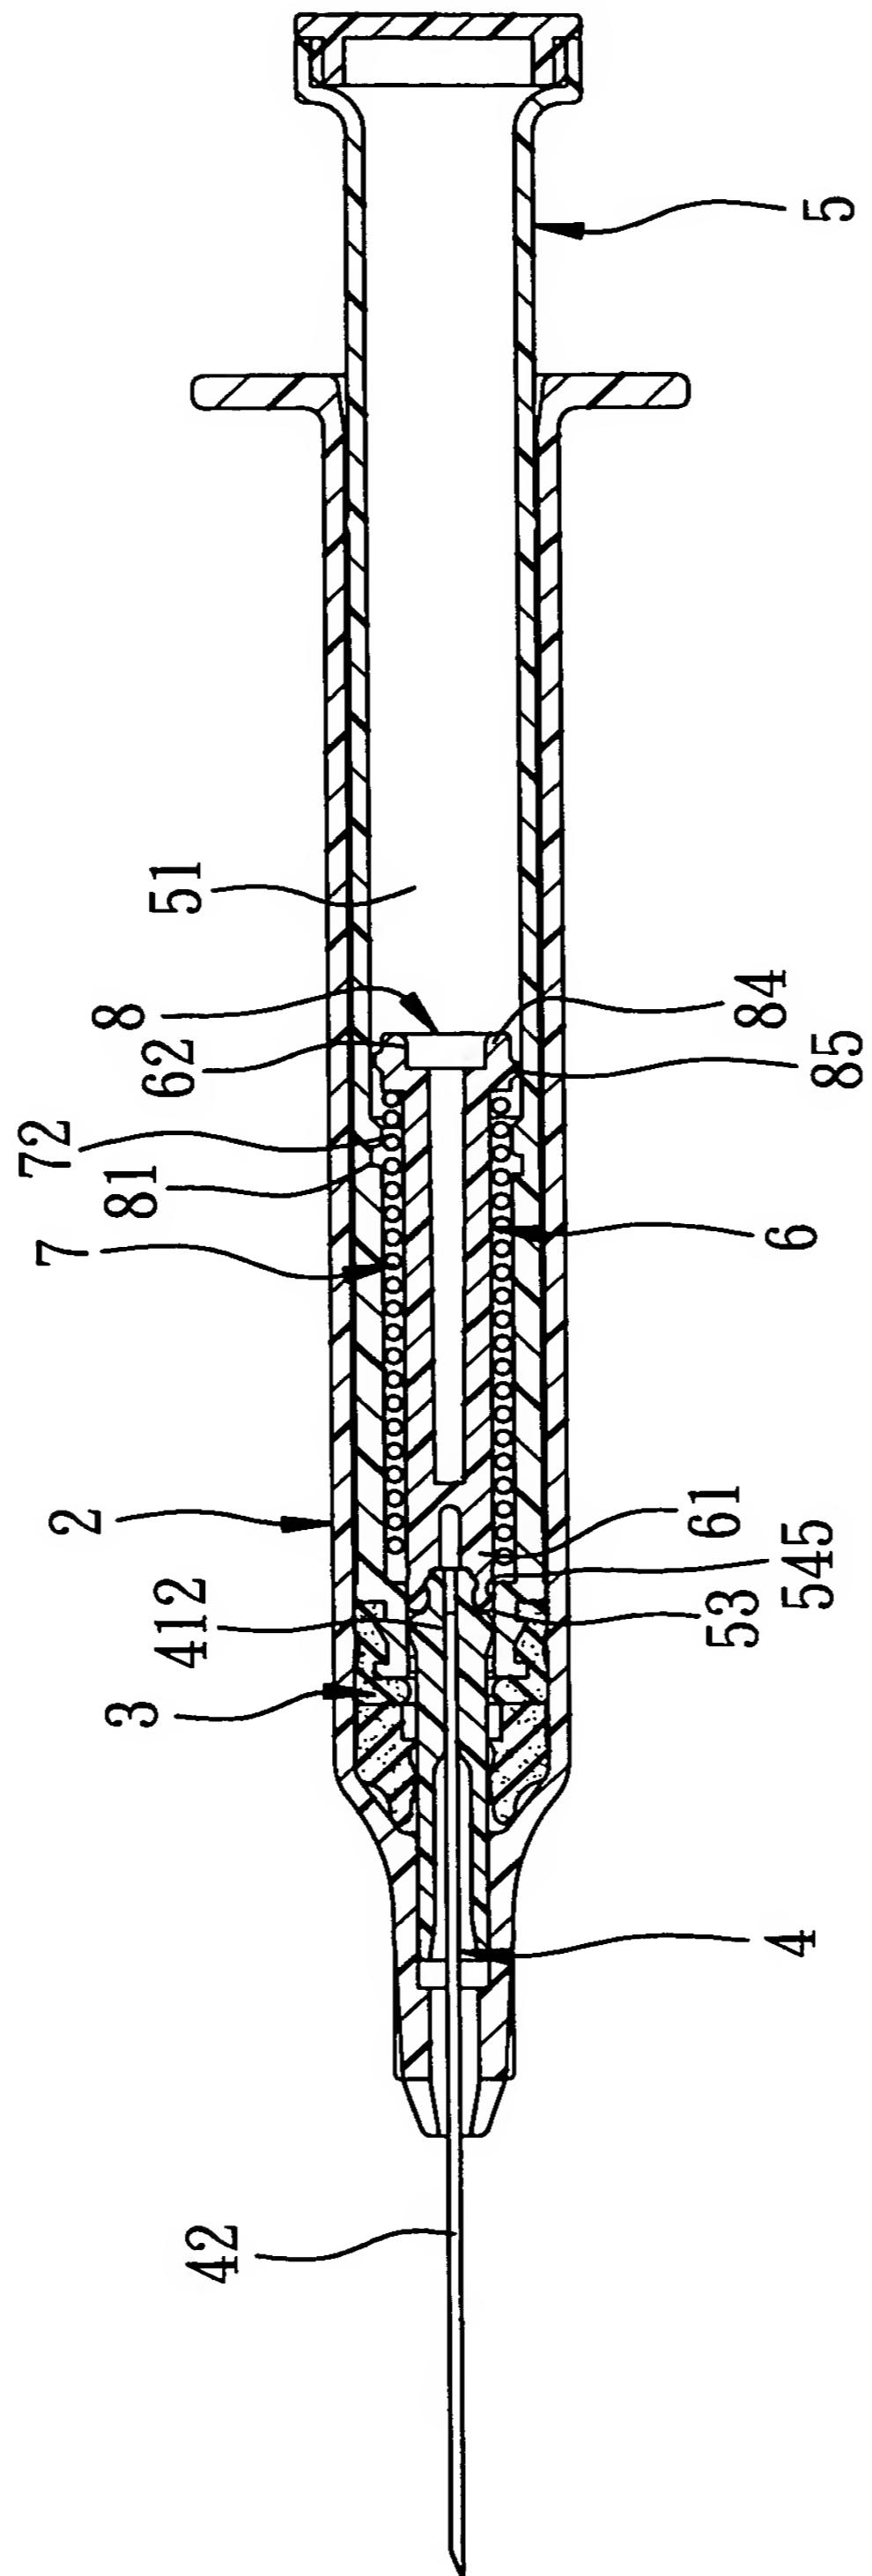


FIG. 11

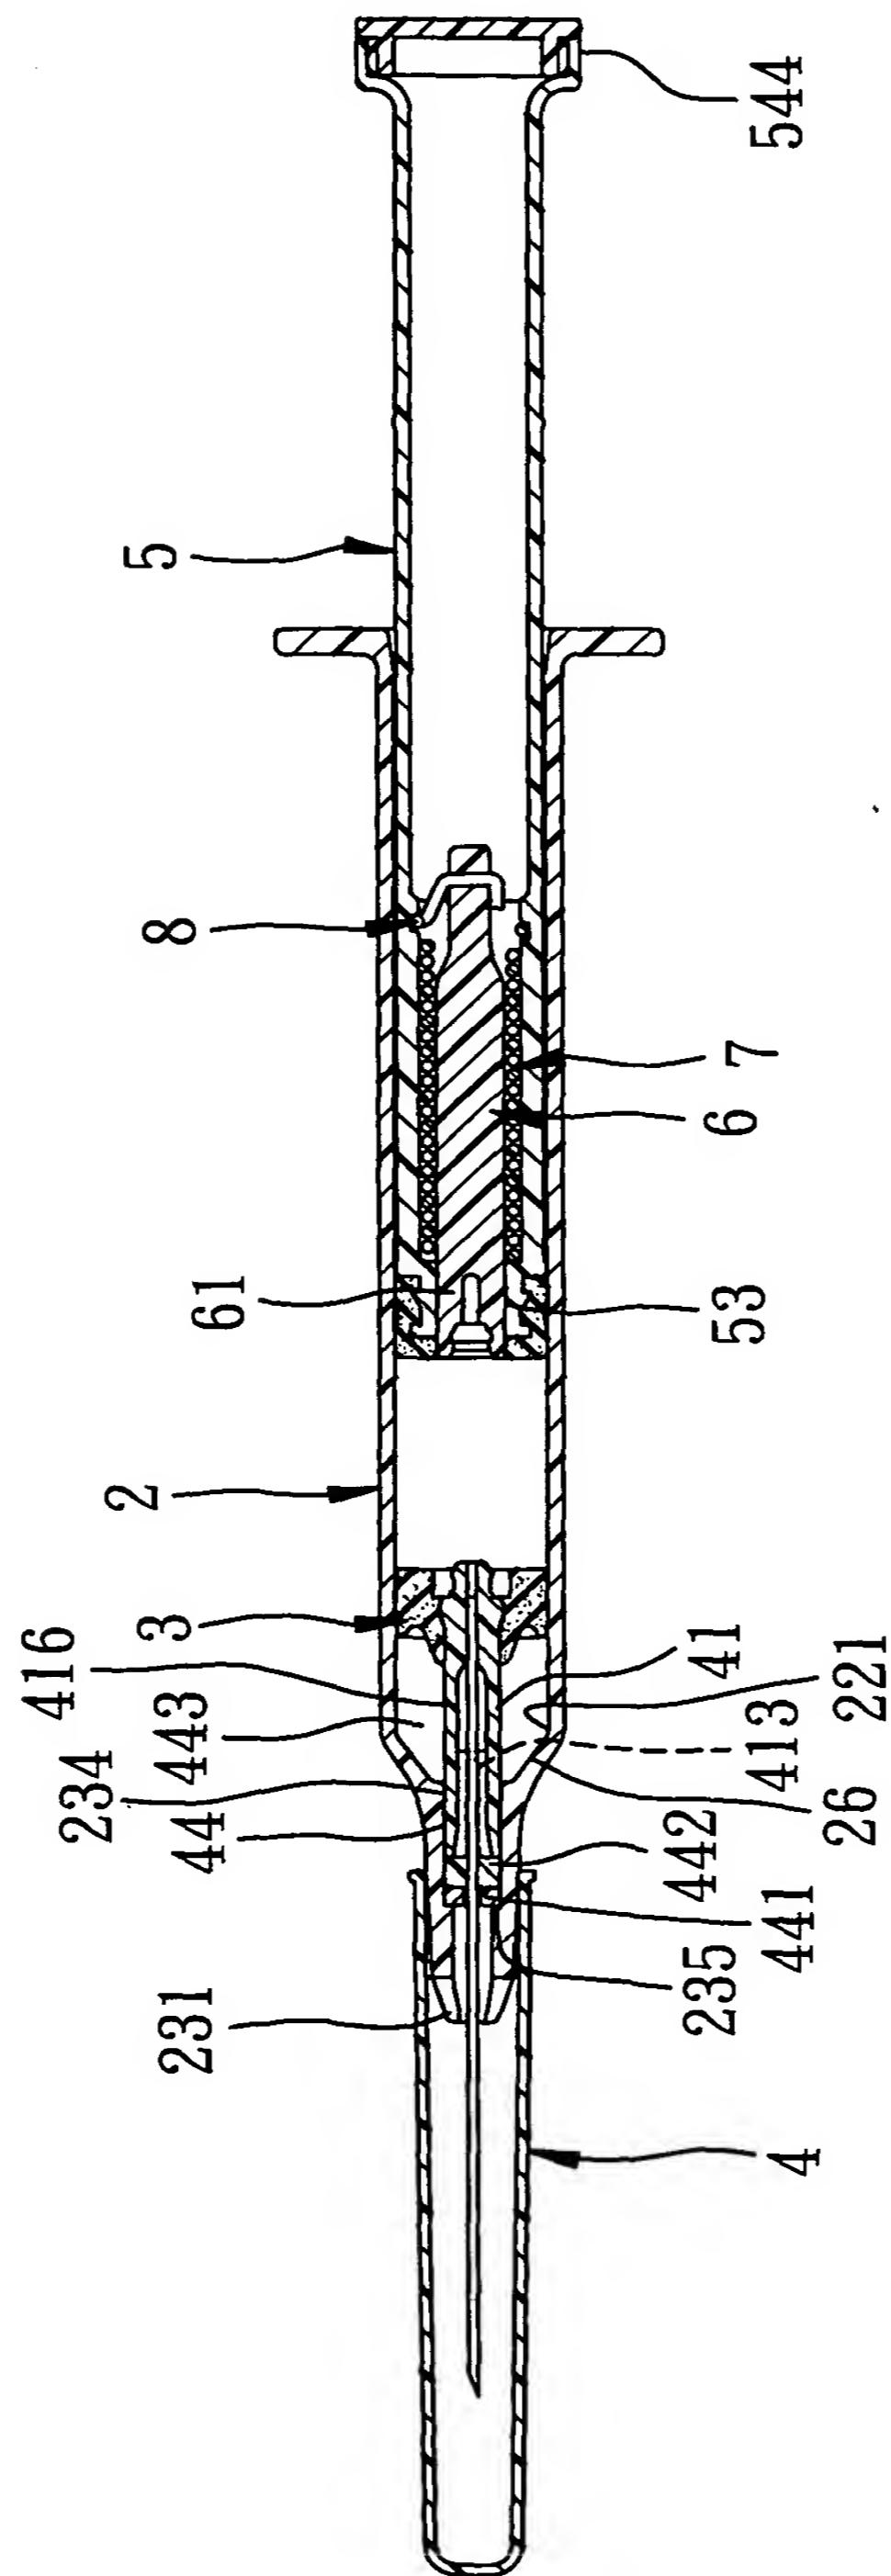


FIG. 12

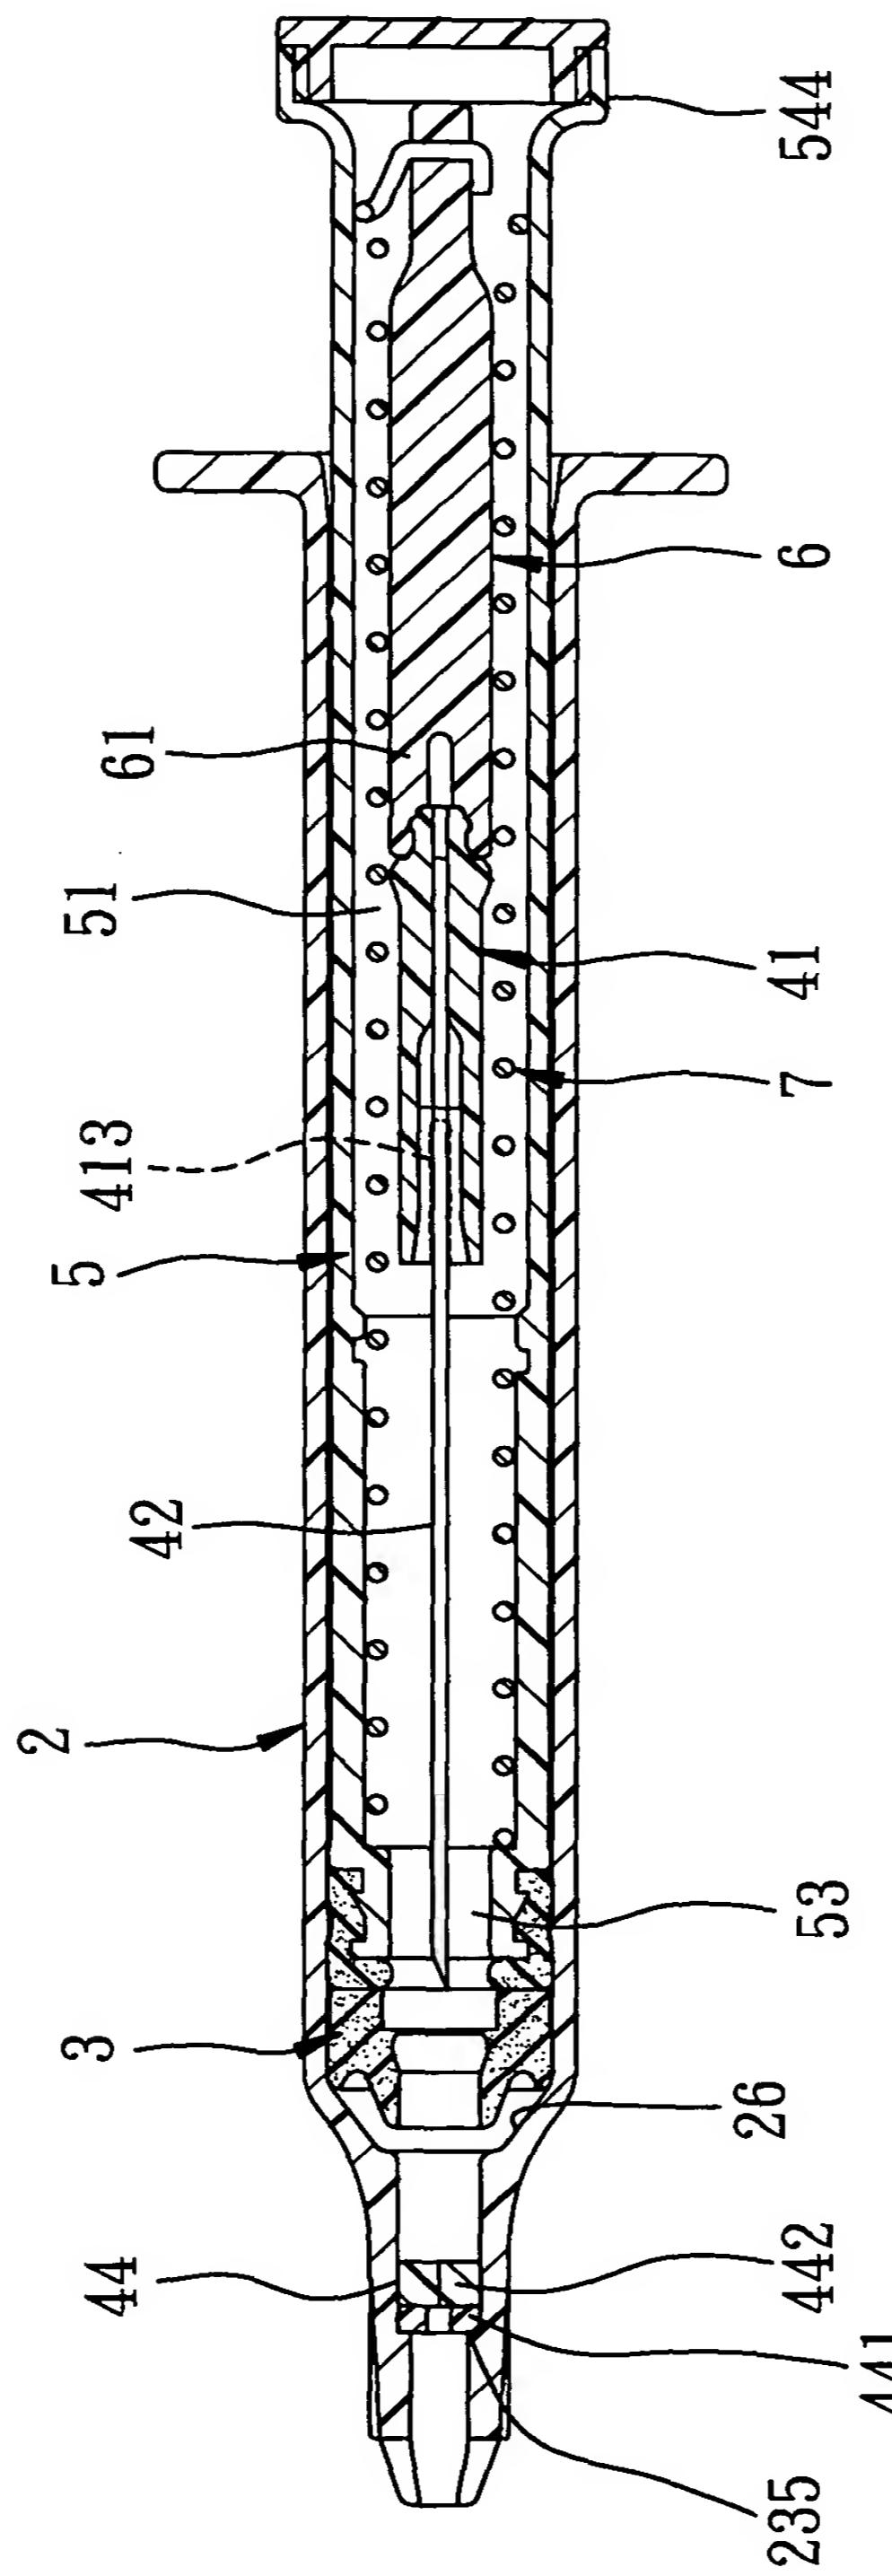


FIG. 13

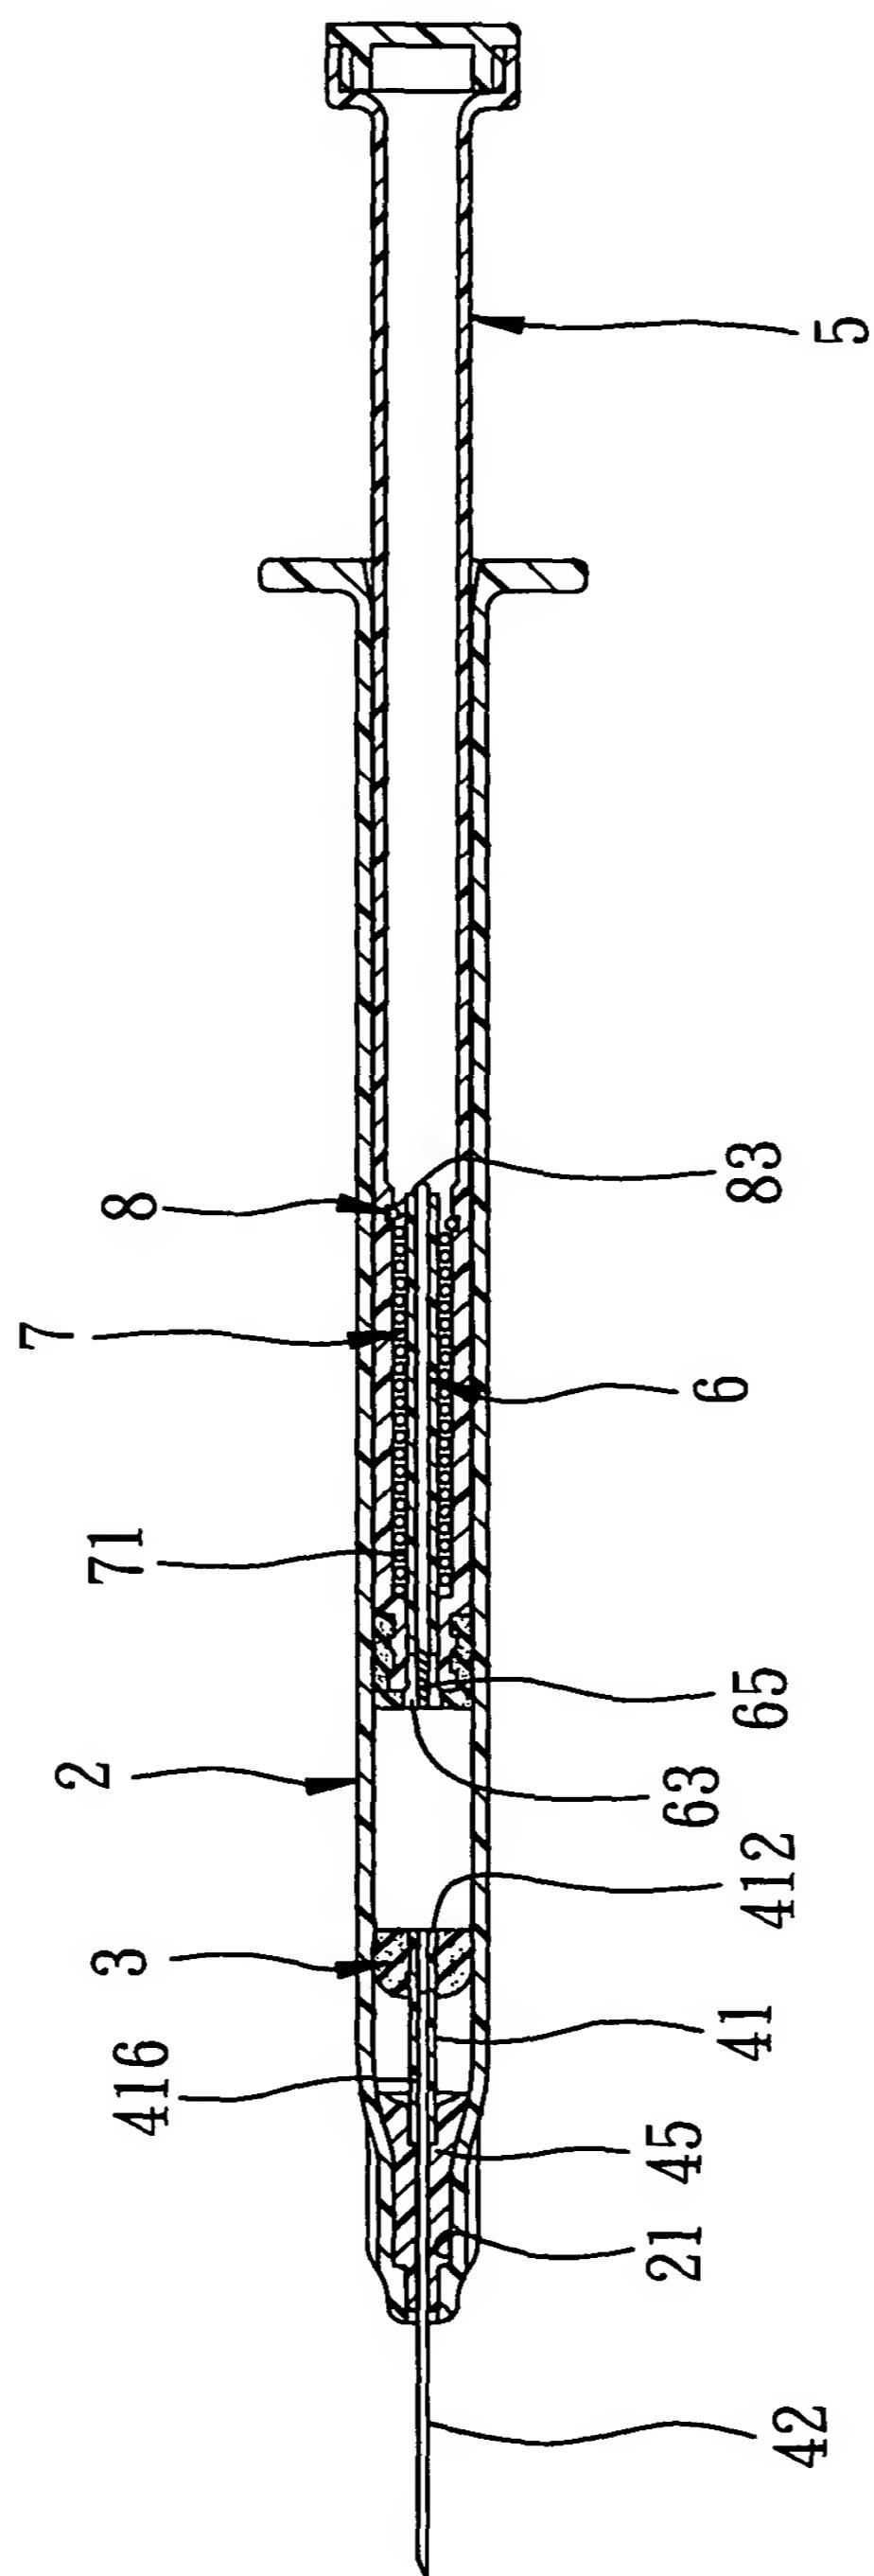


FIG. 14

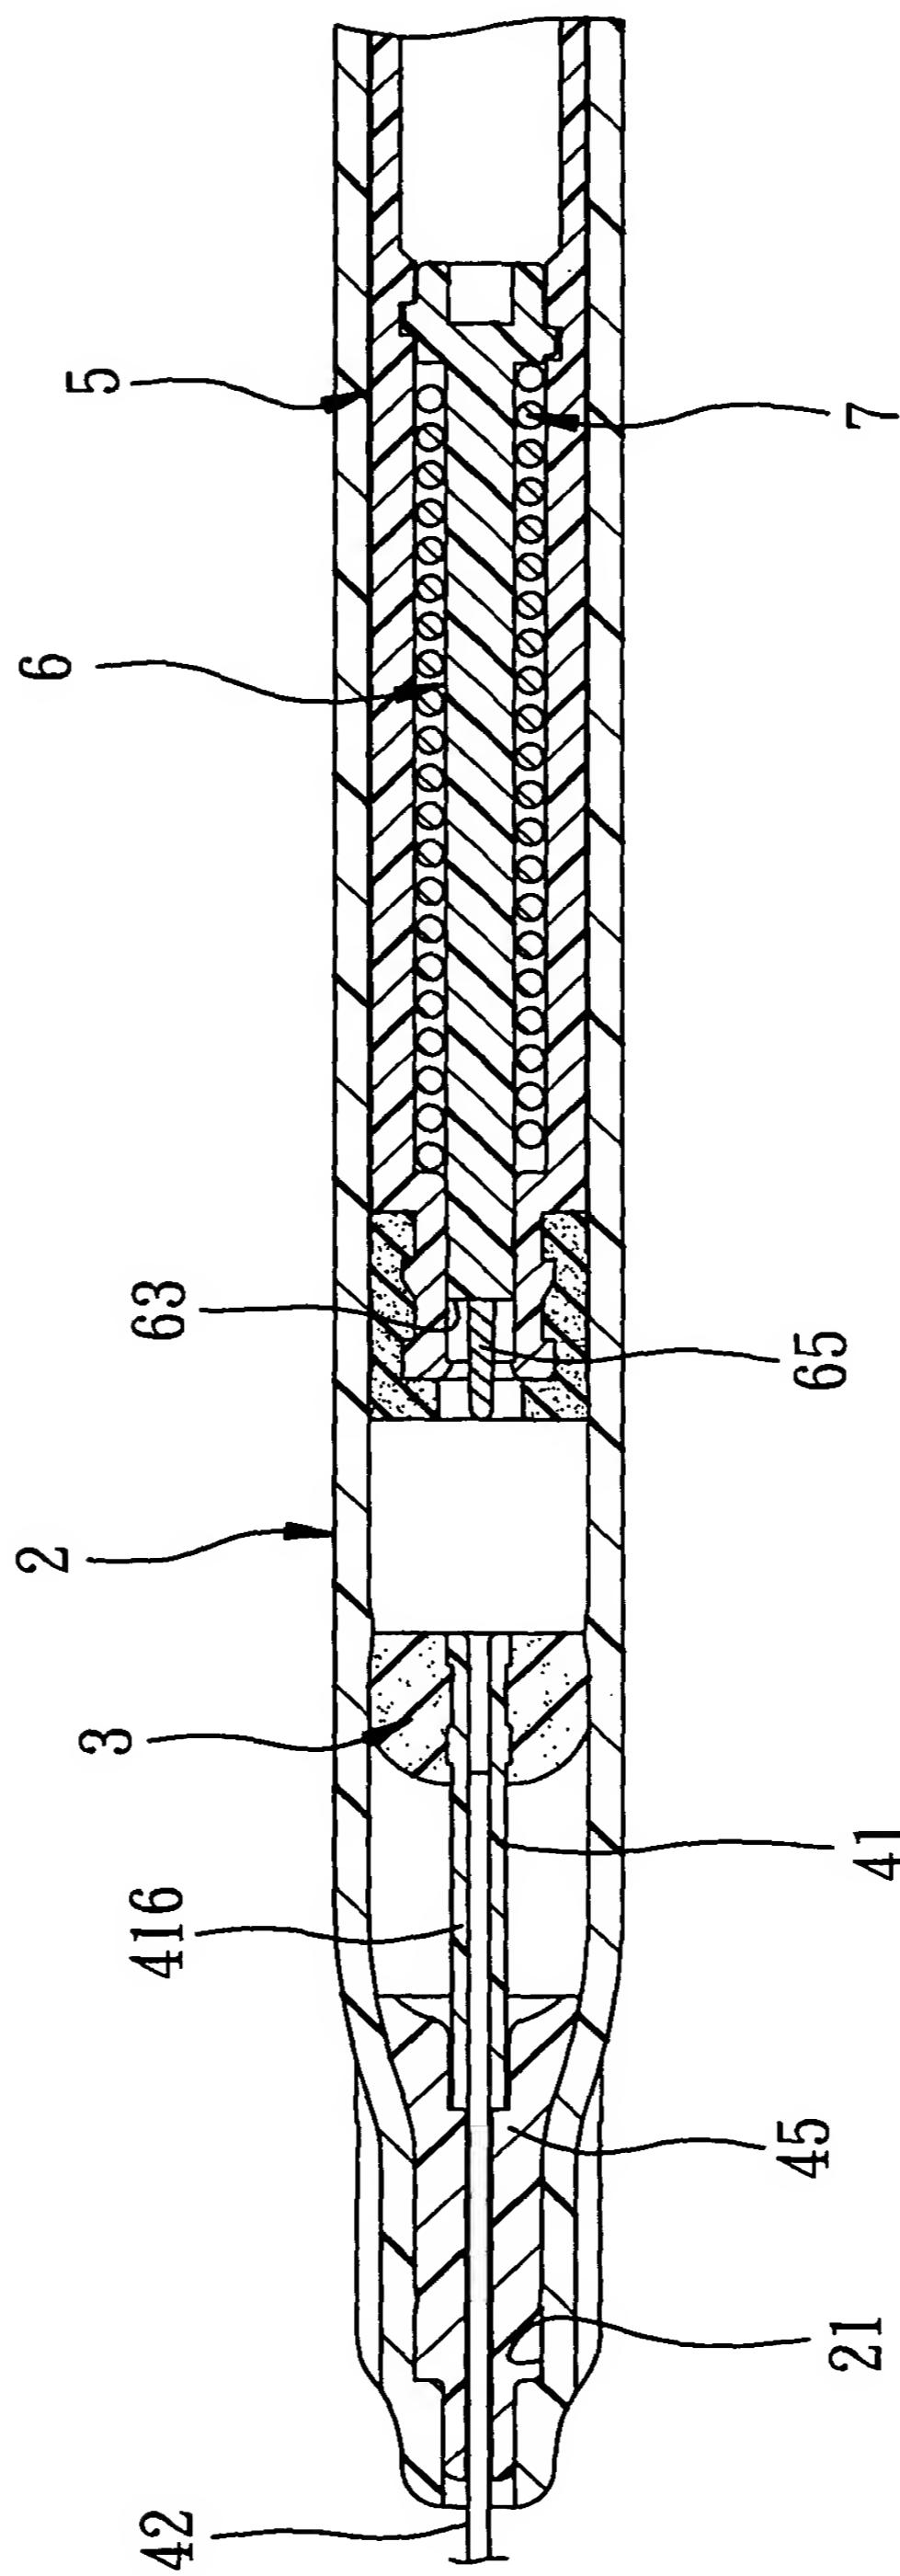


FIG. 15

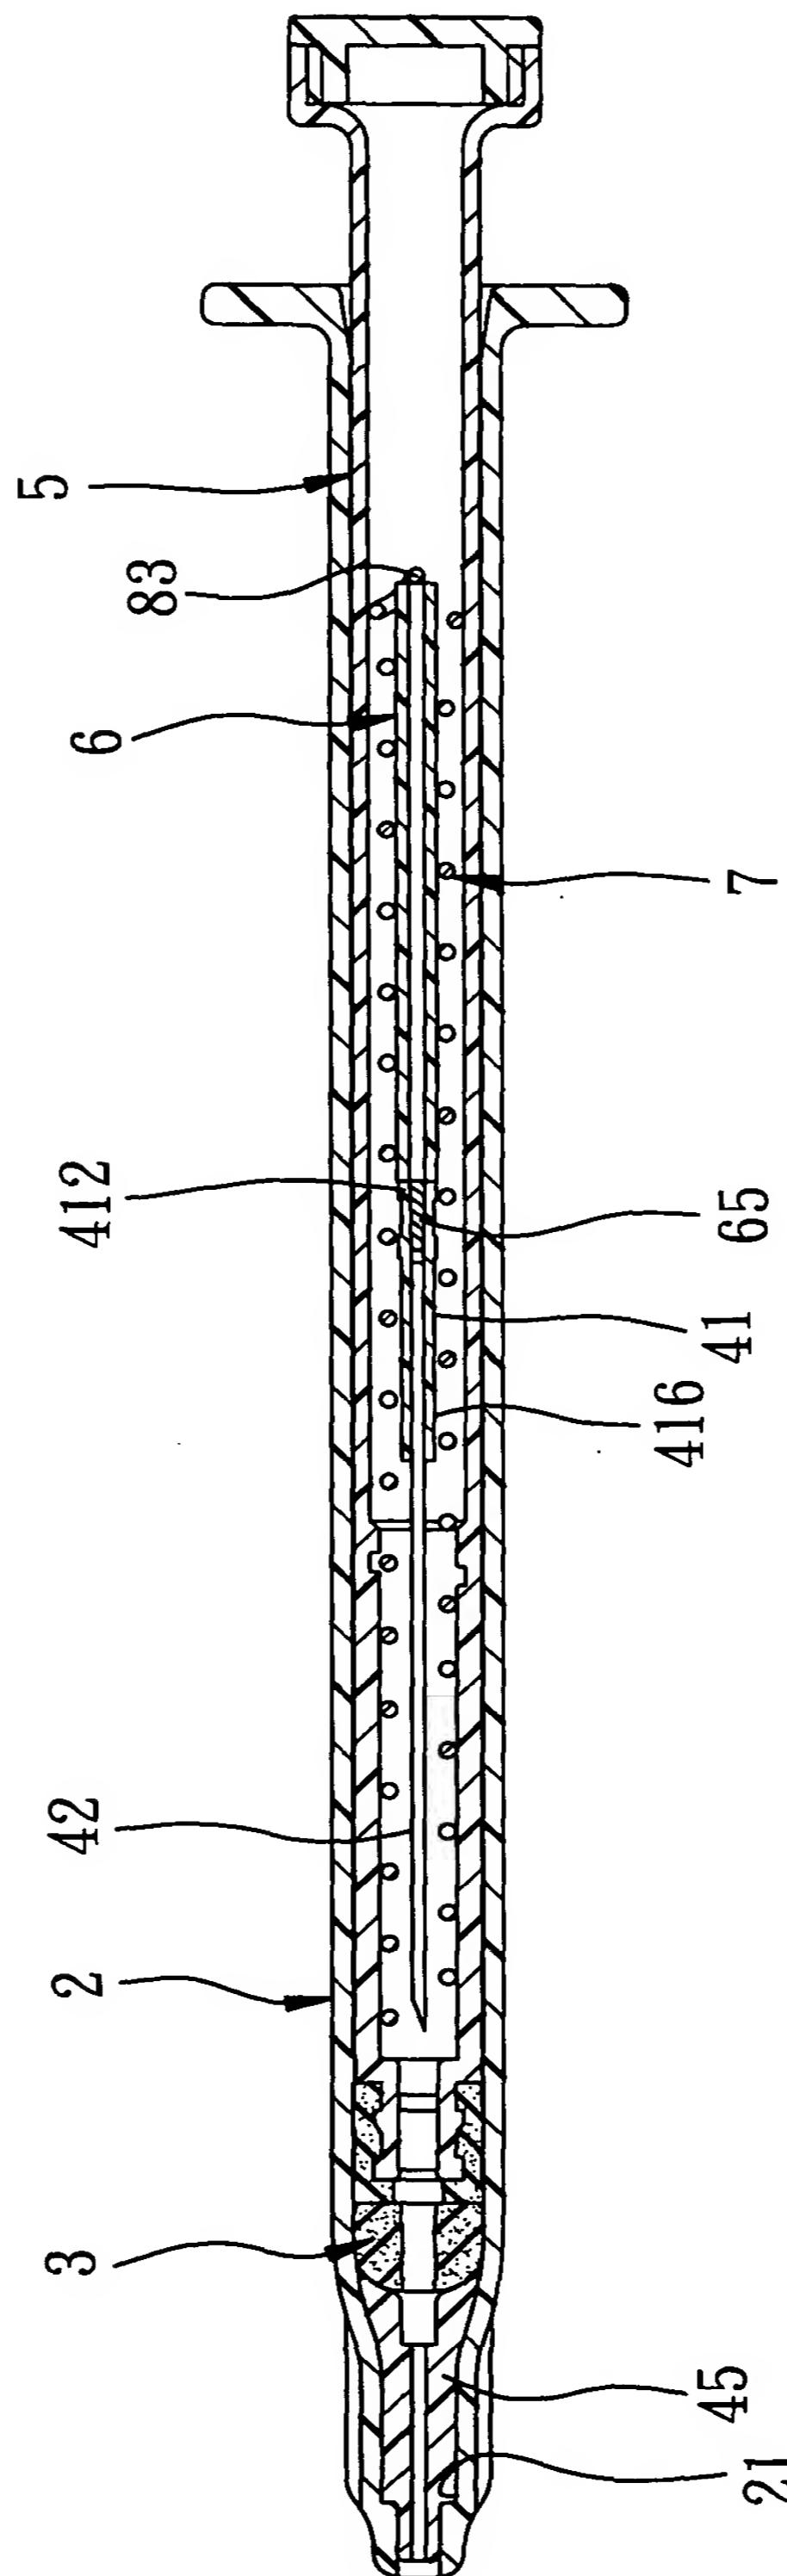


FIG. 16

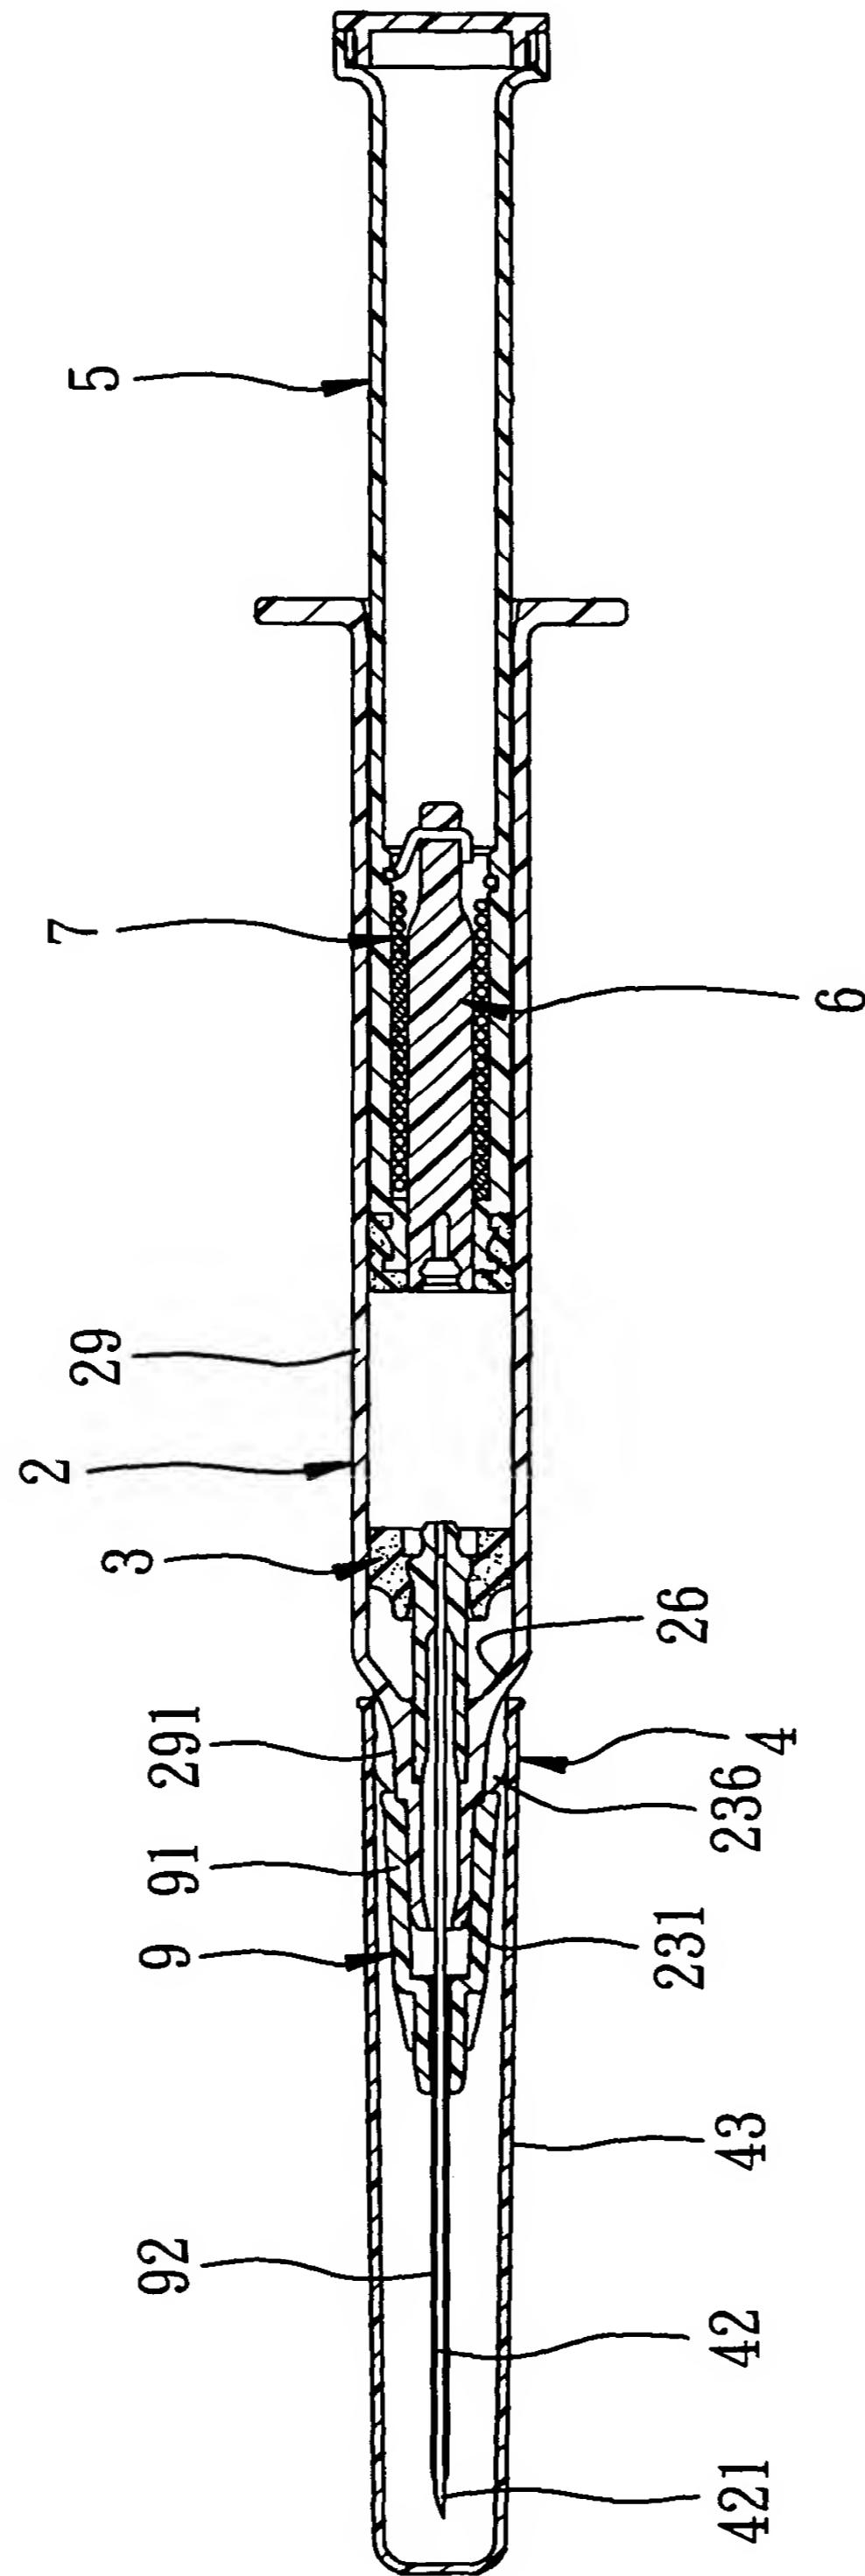


FIG. 17

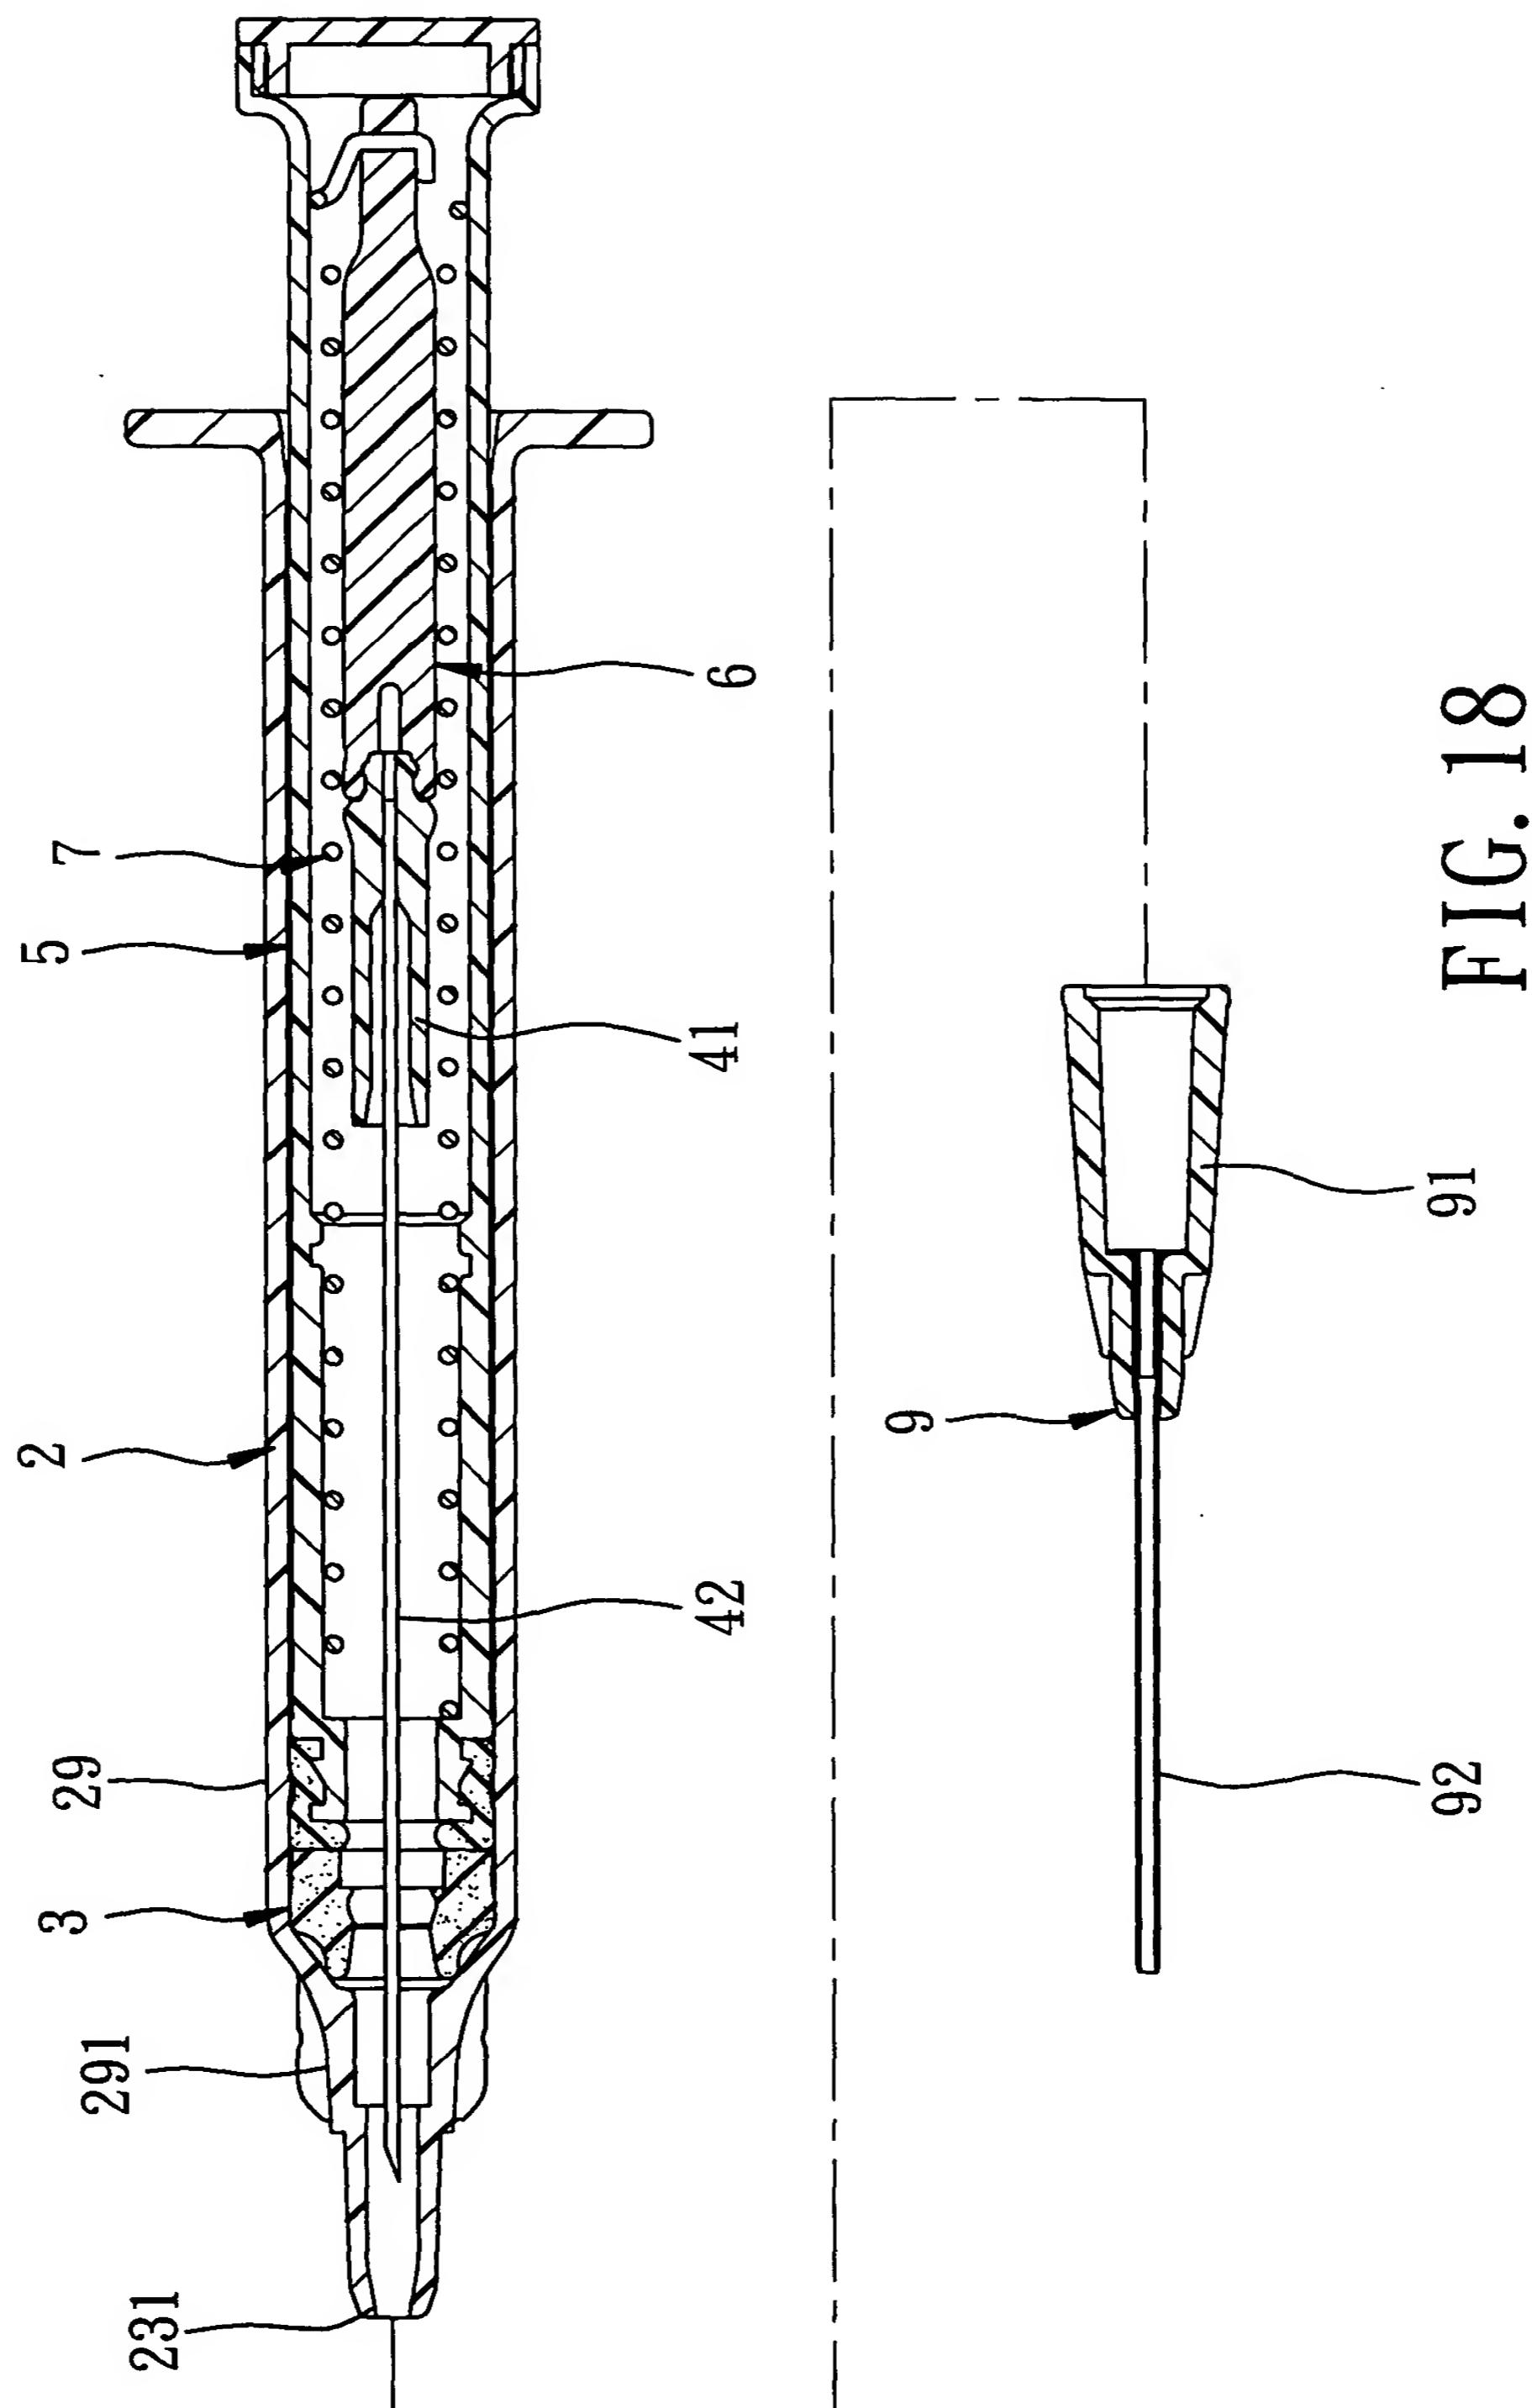


FIG. 18

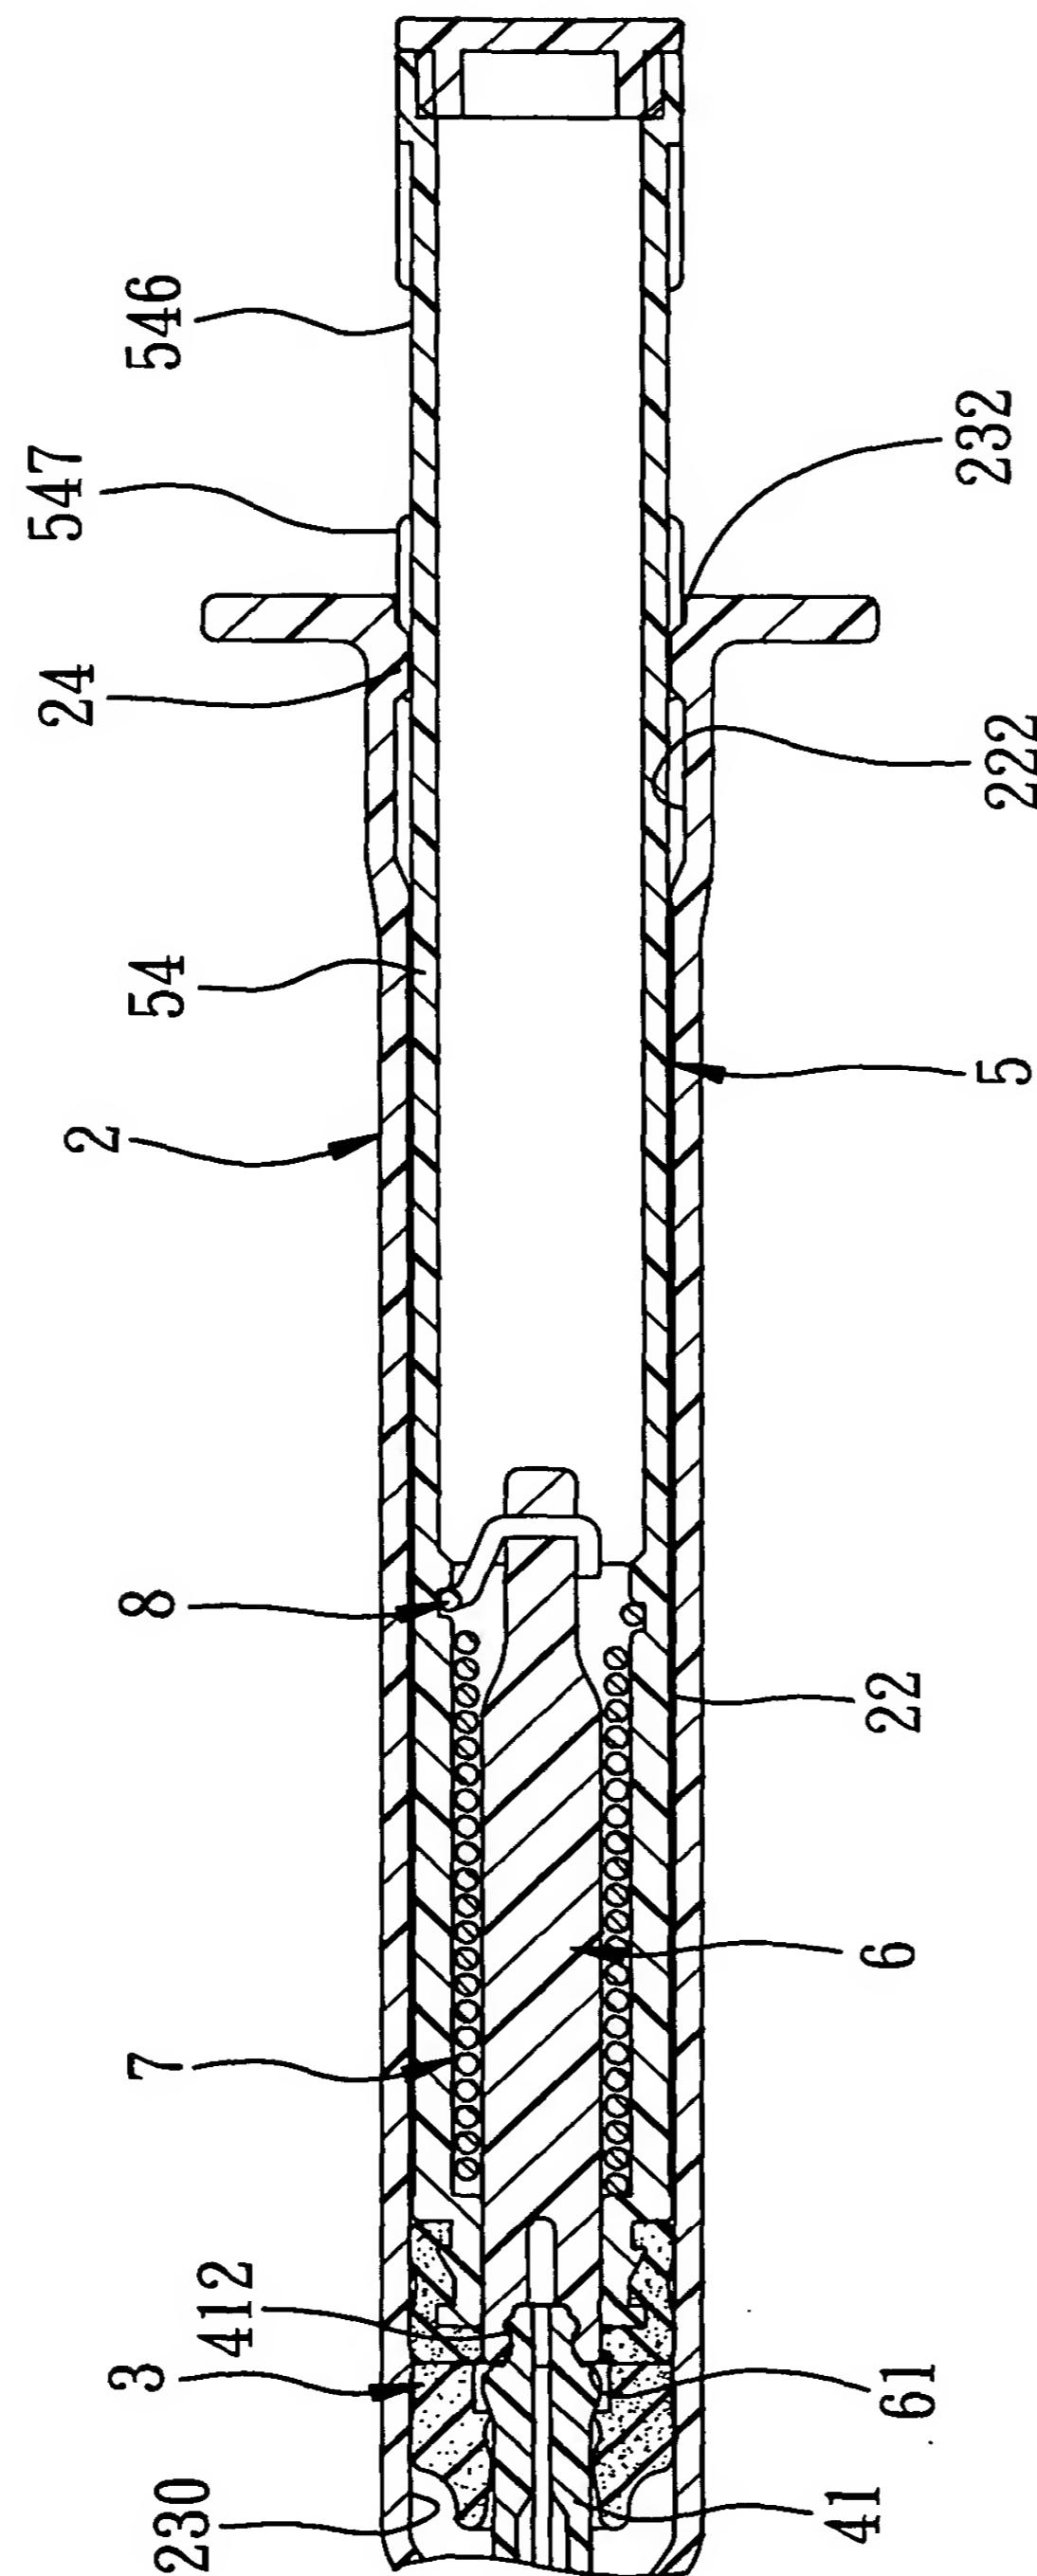


FIG. 19

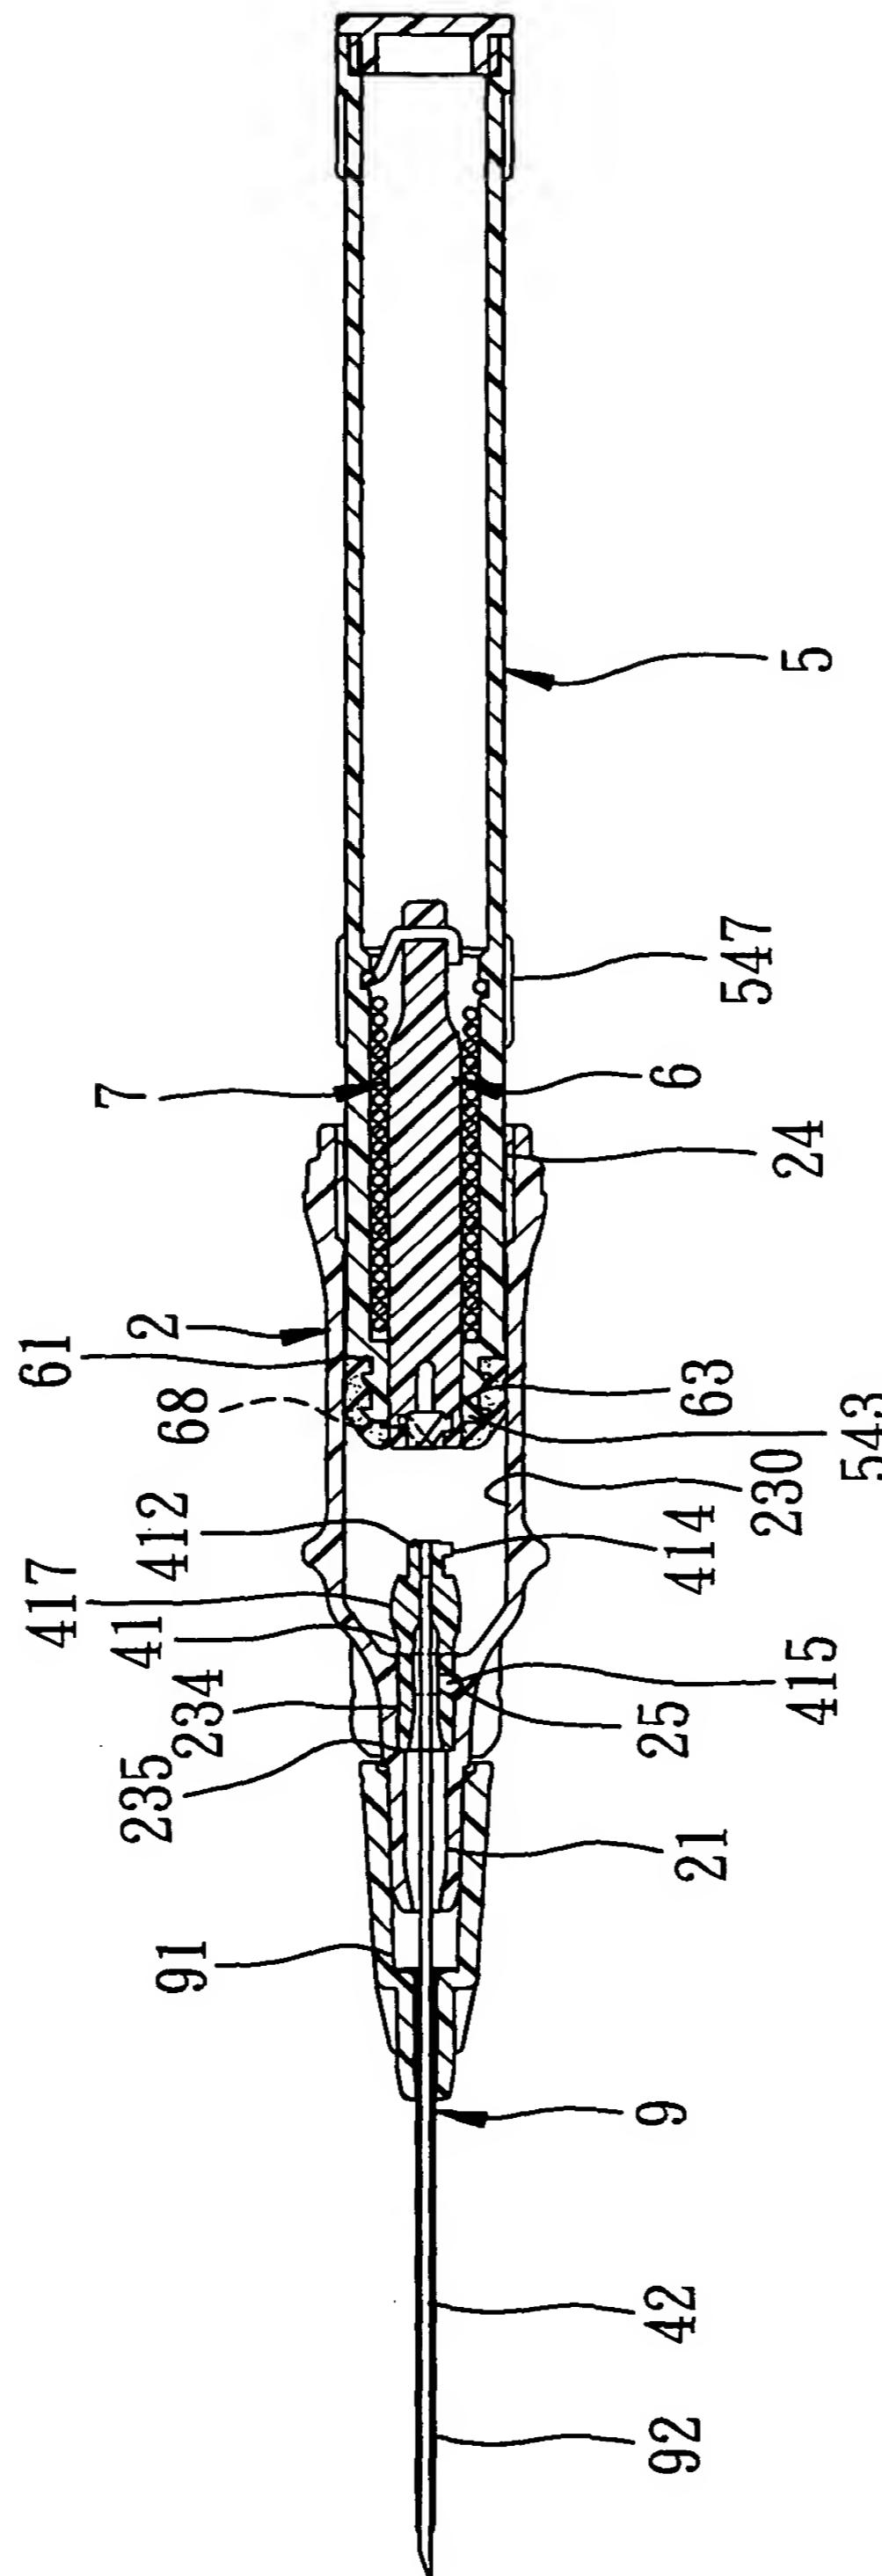


FIG. 20

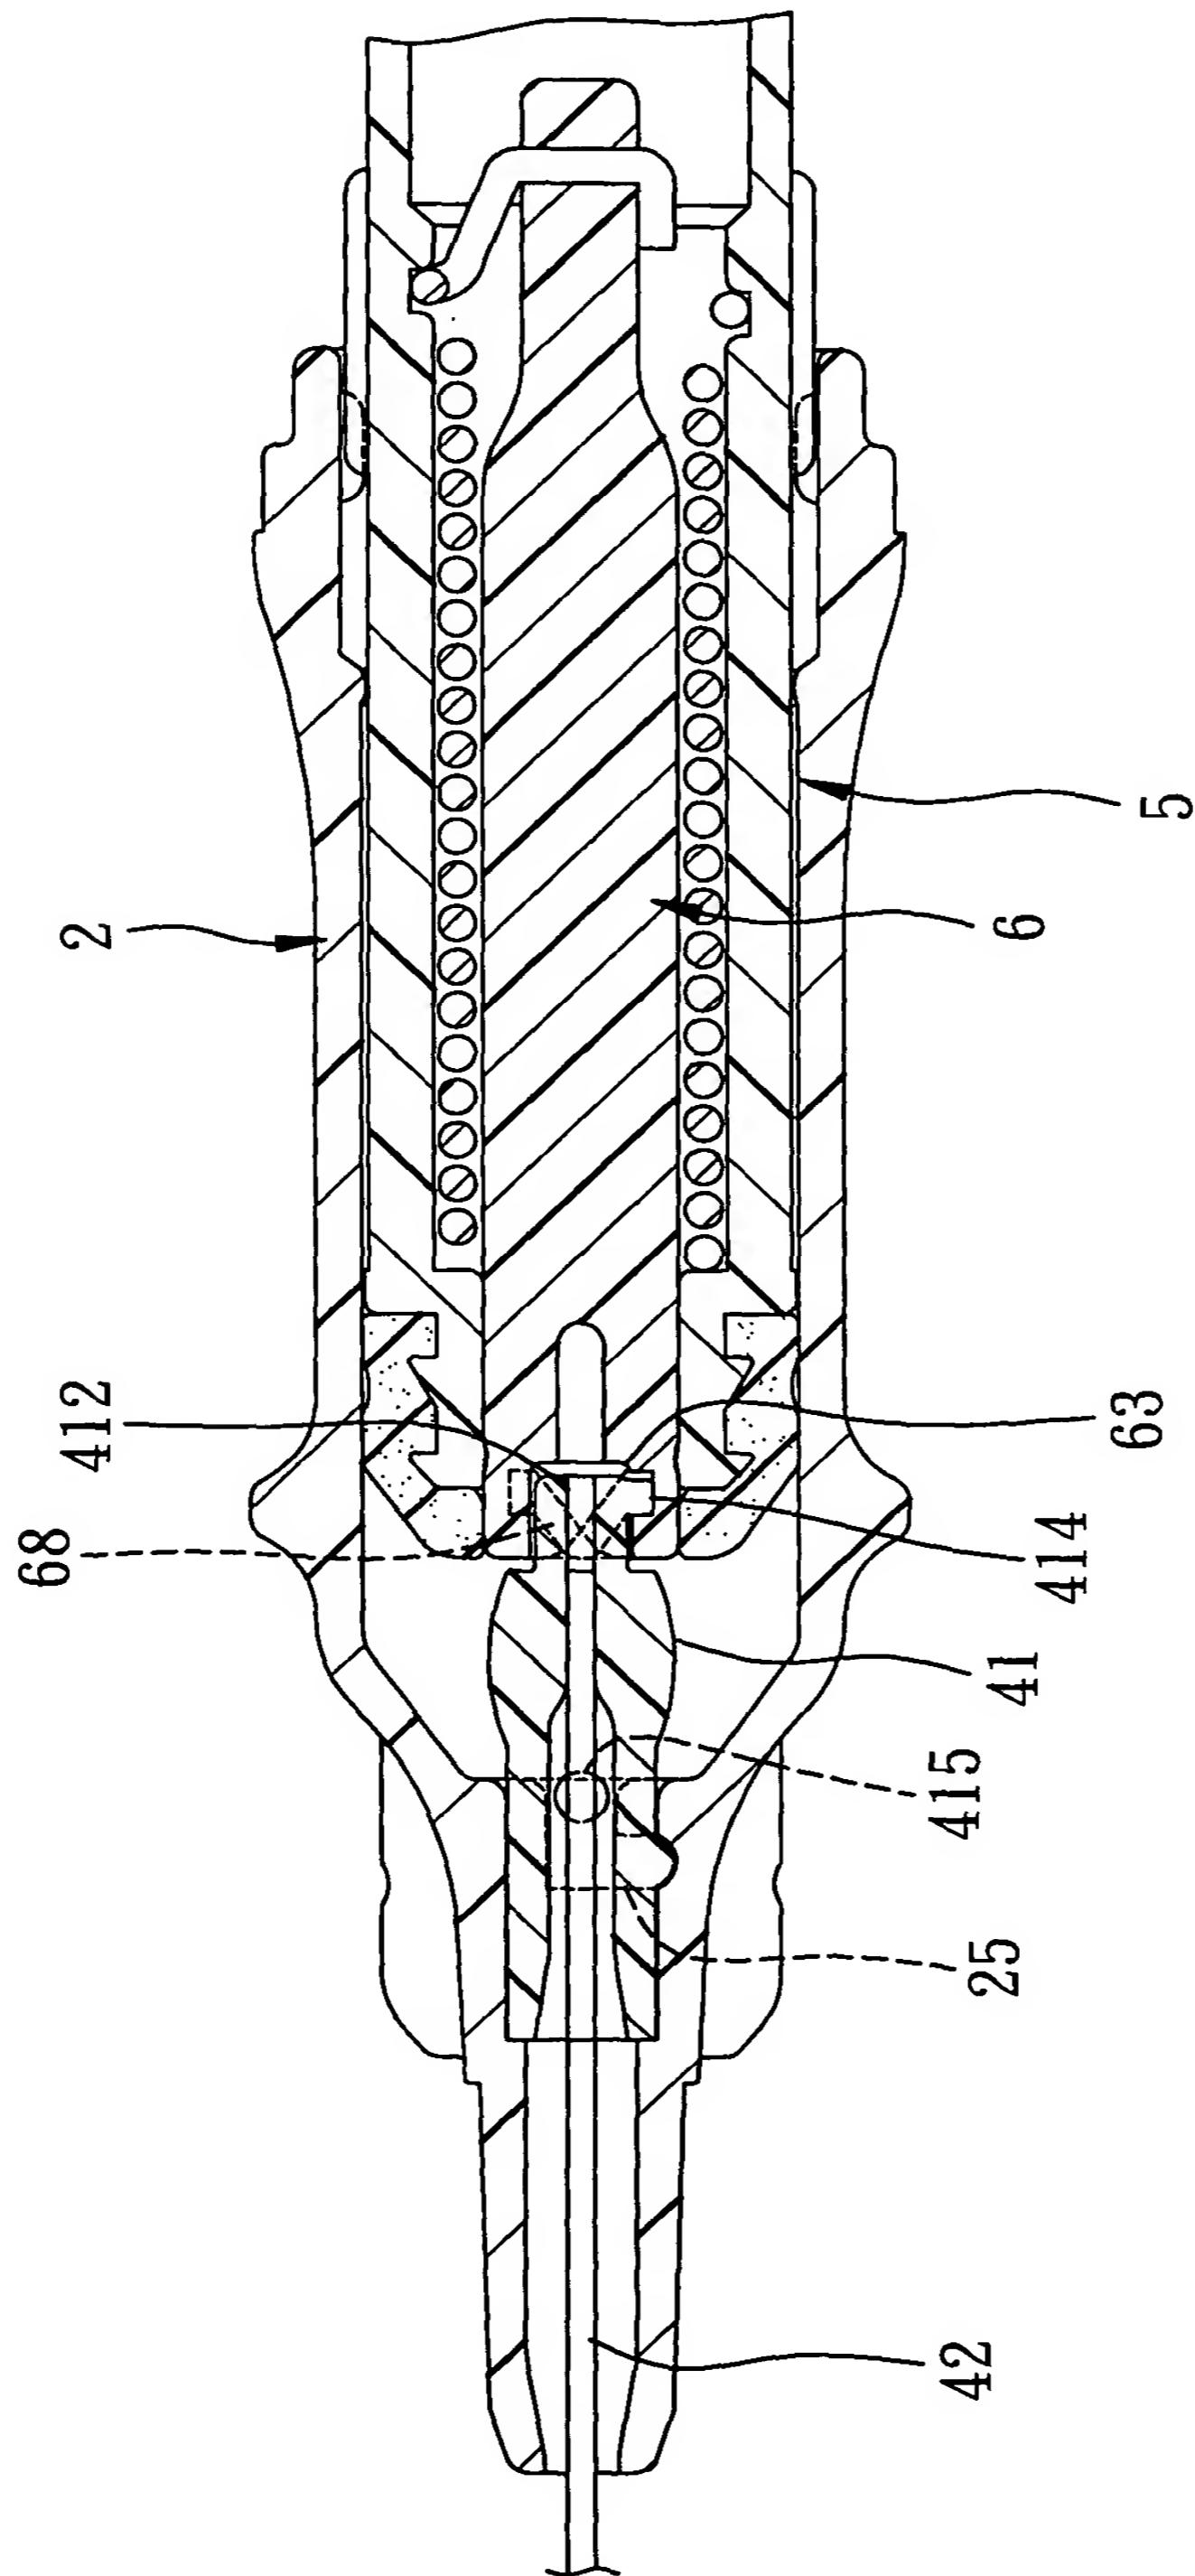


FIG. 21

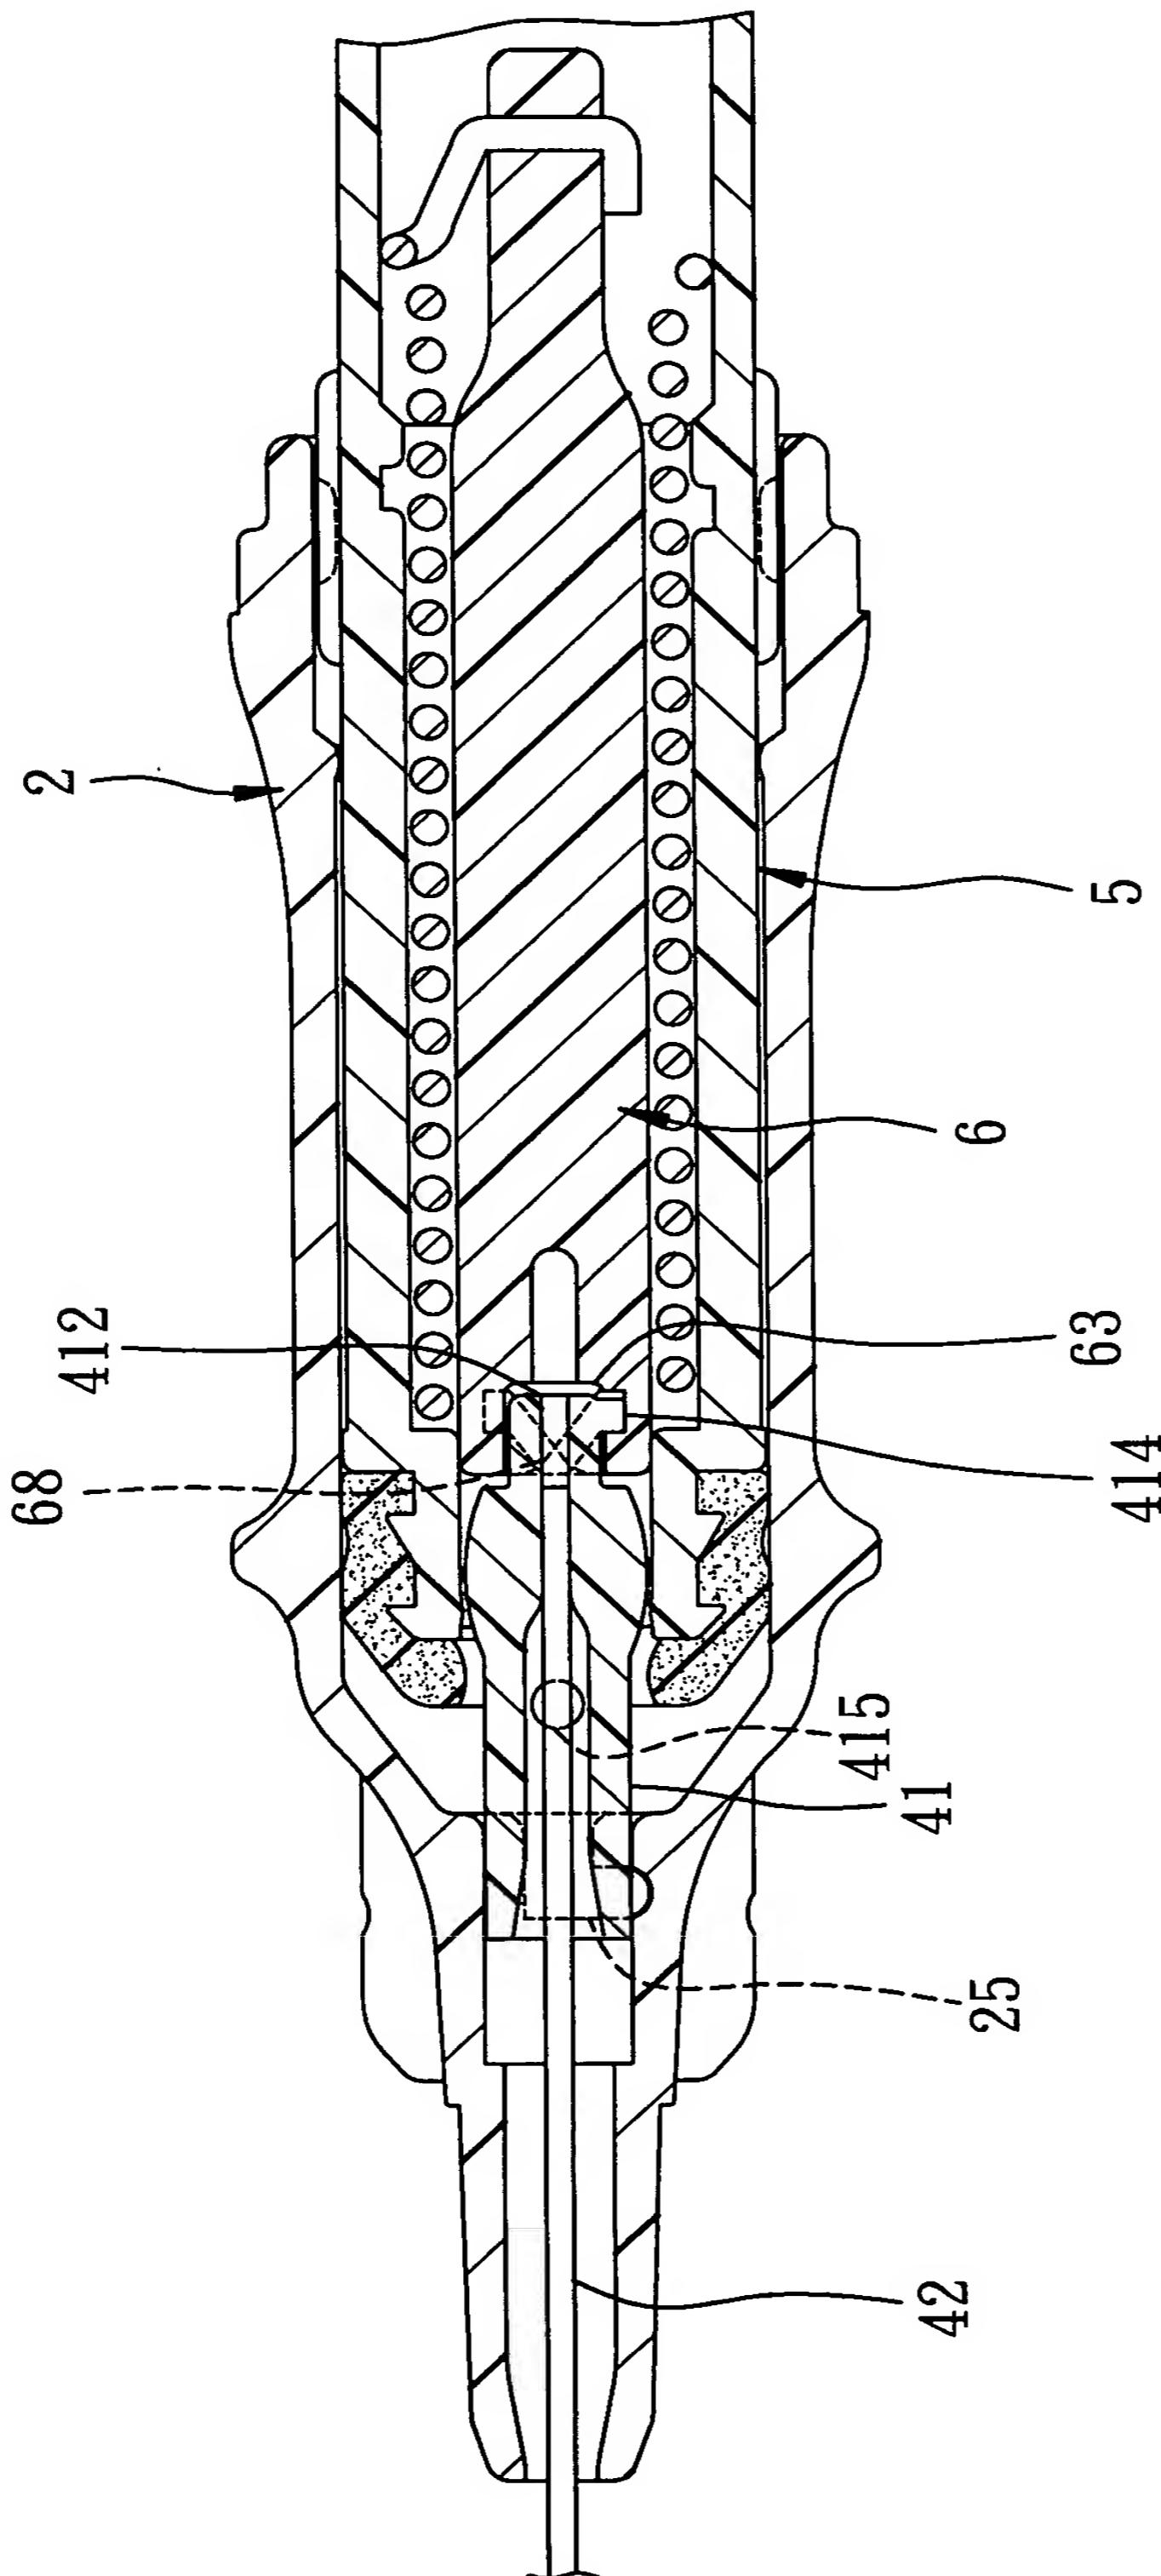


FIG. 22

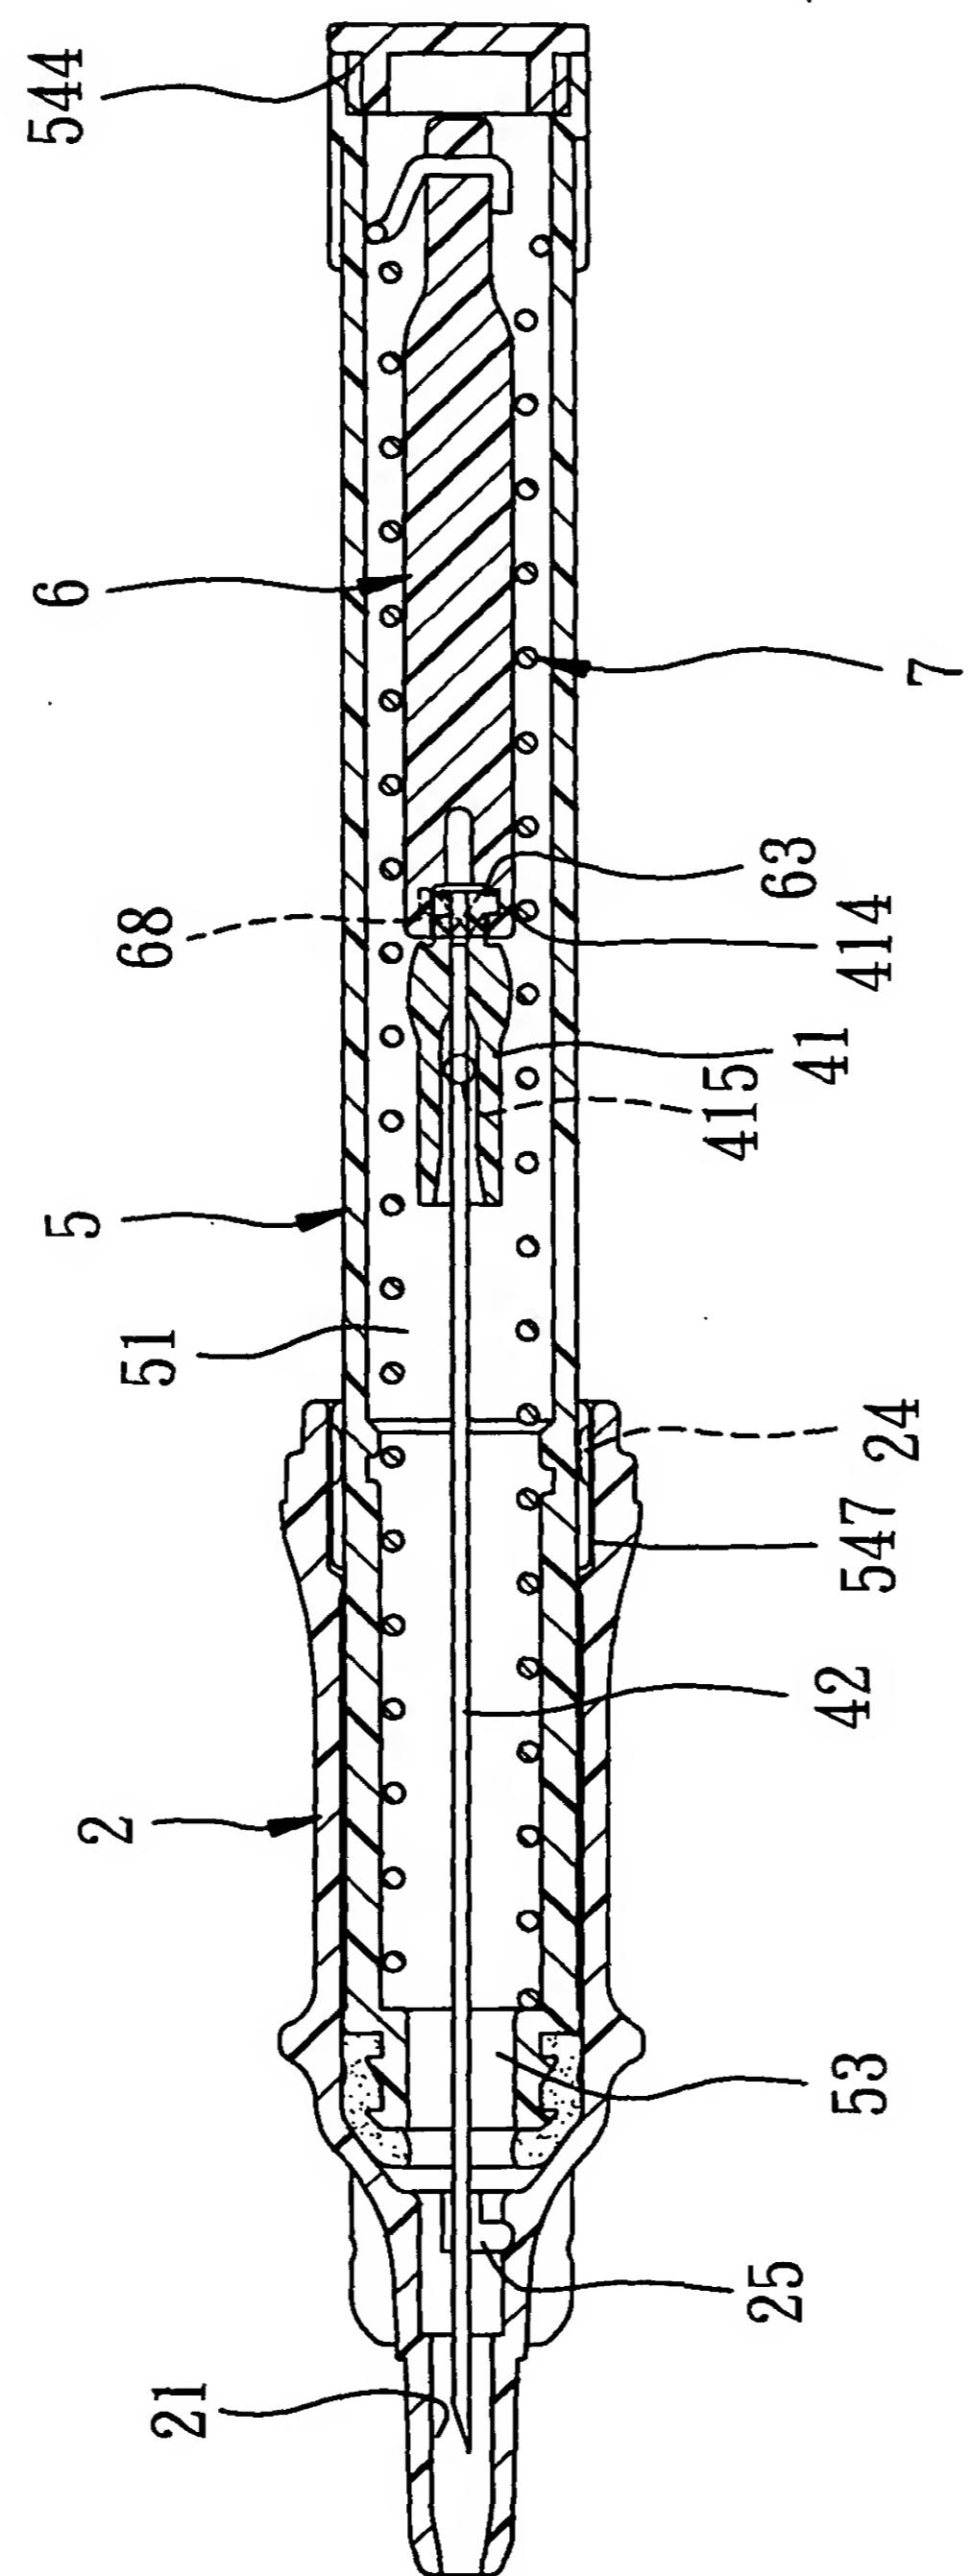


FIG. 23

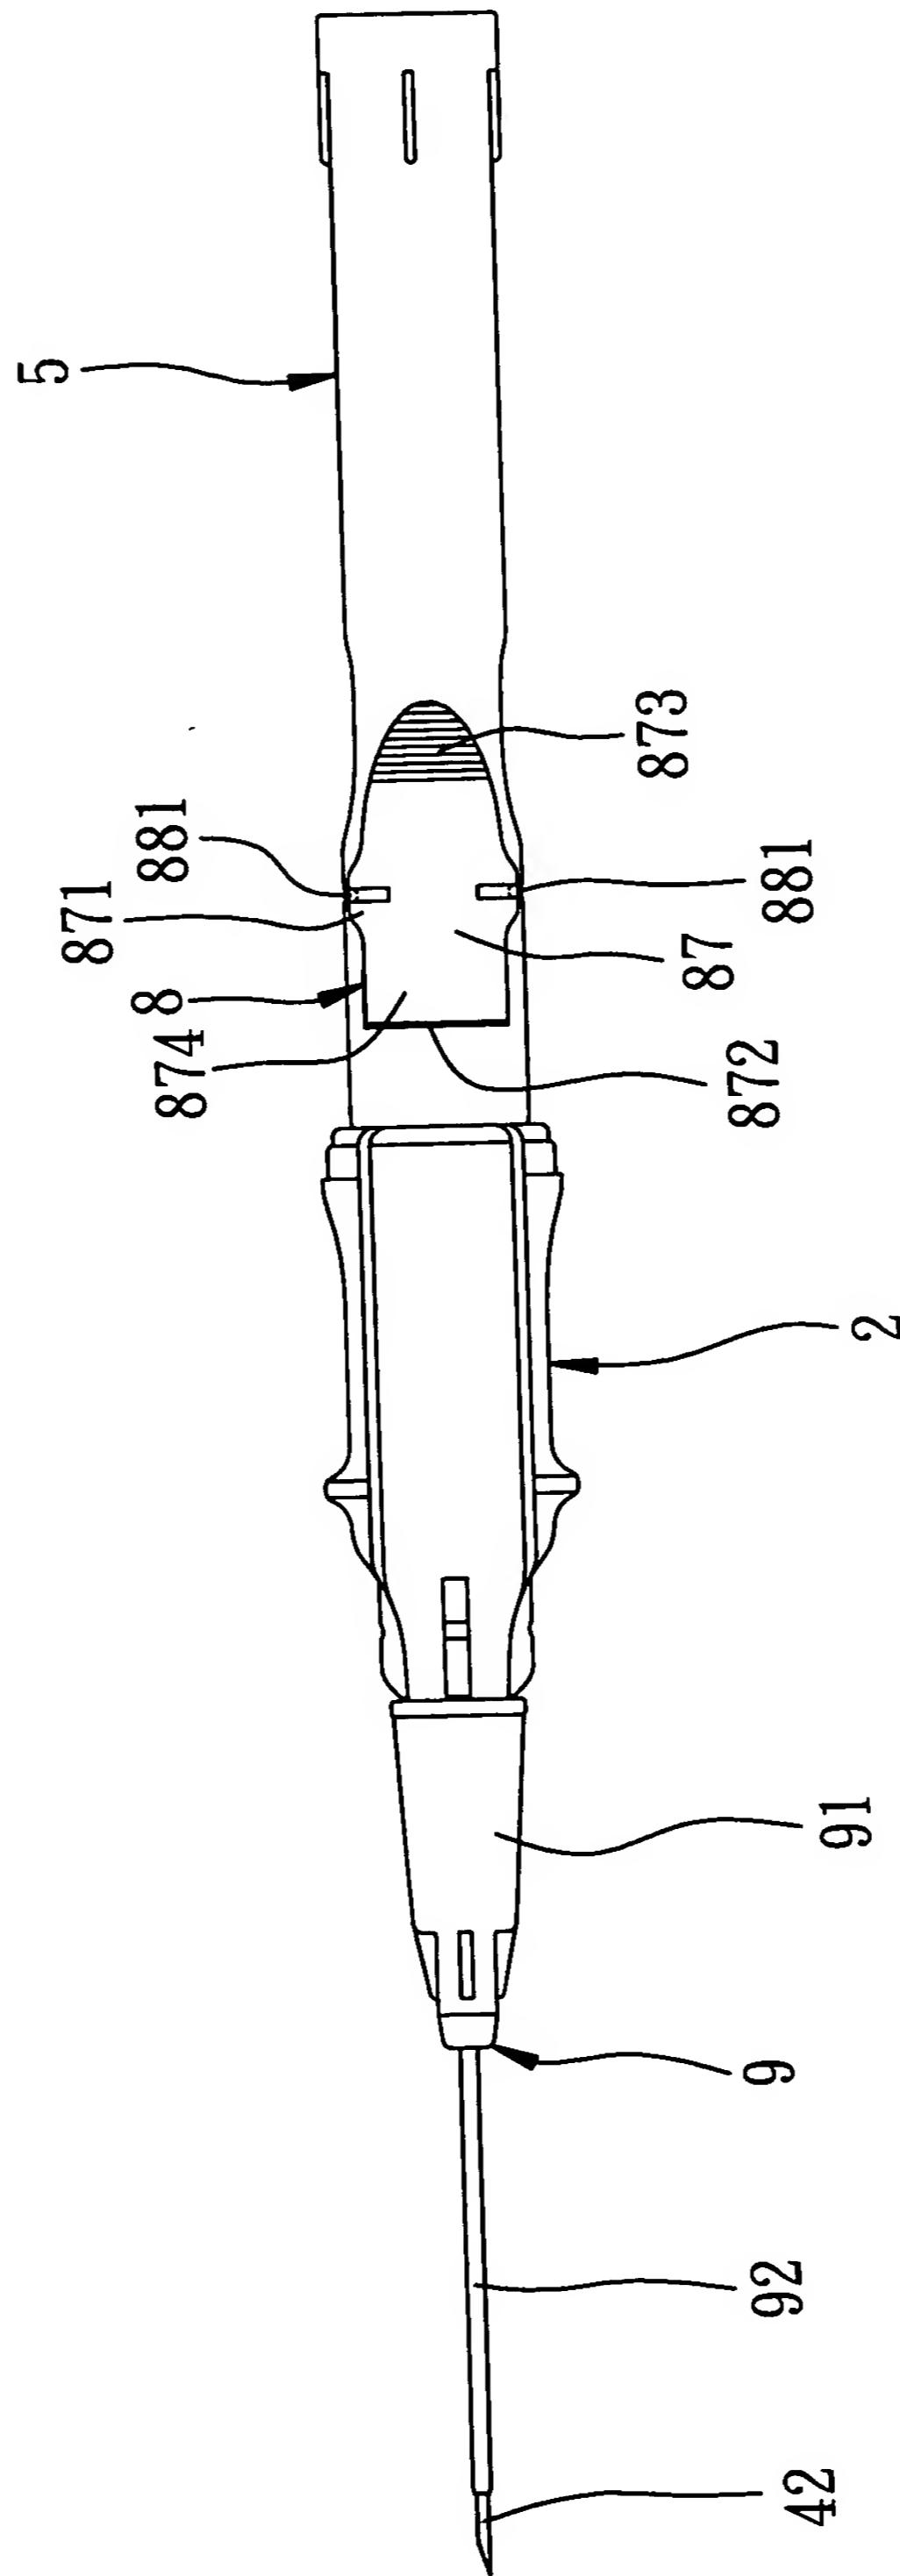


FIG. 24

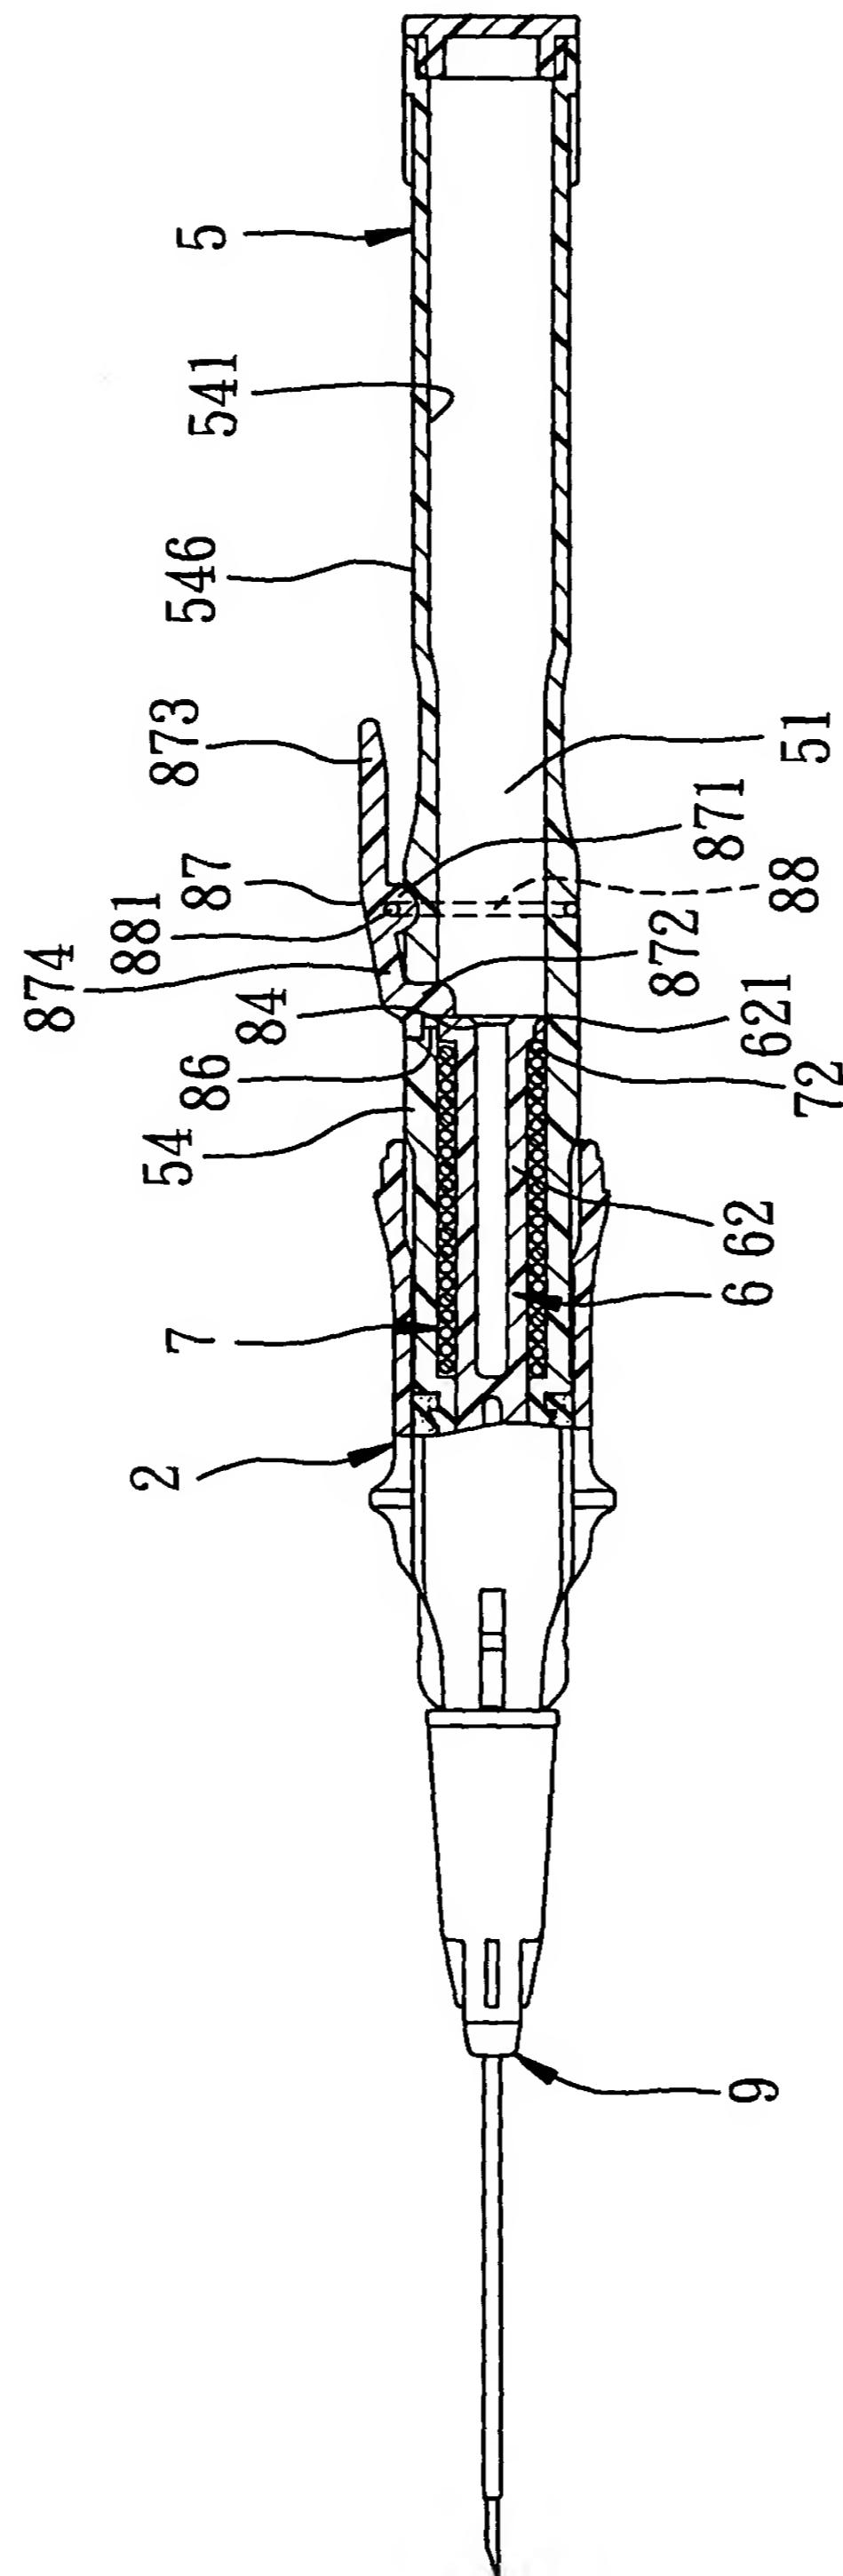


FIG. 25

DISPOSABLE SYRINGE
Shue et al. Filed Sept. 22, 2003 Docket #48006-4

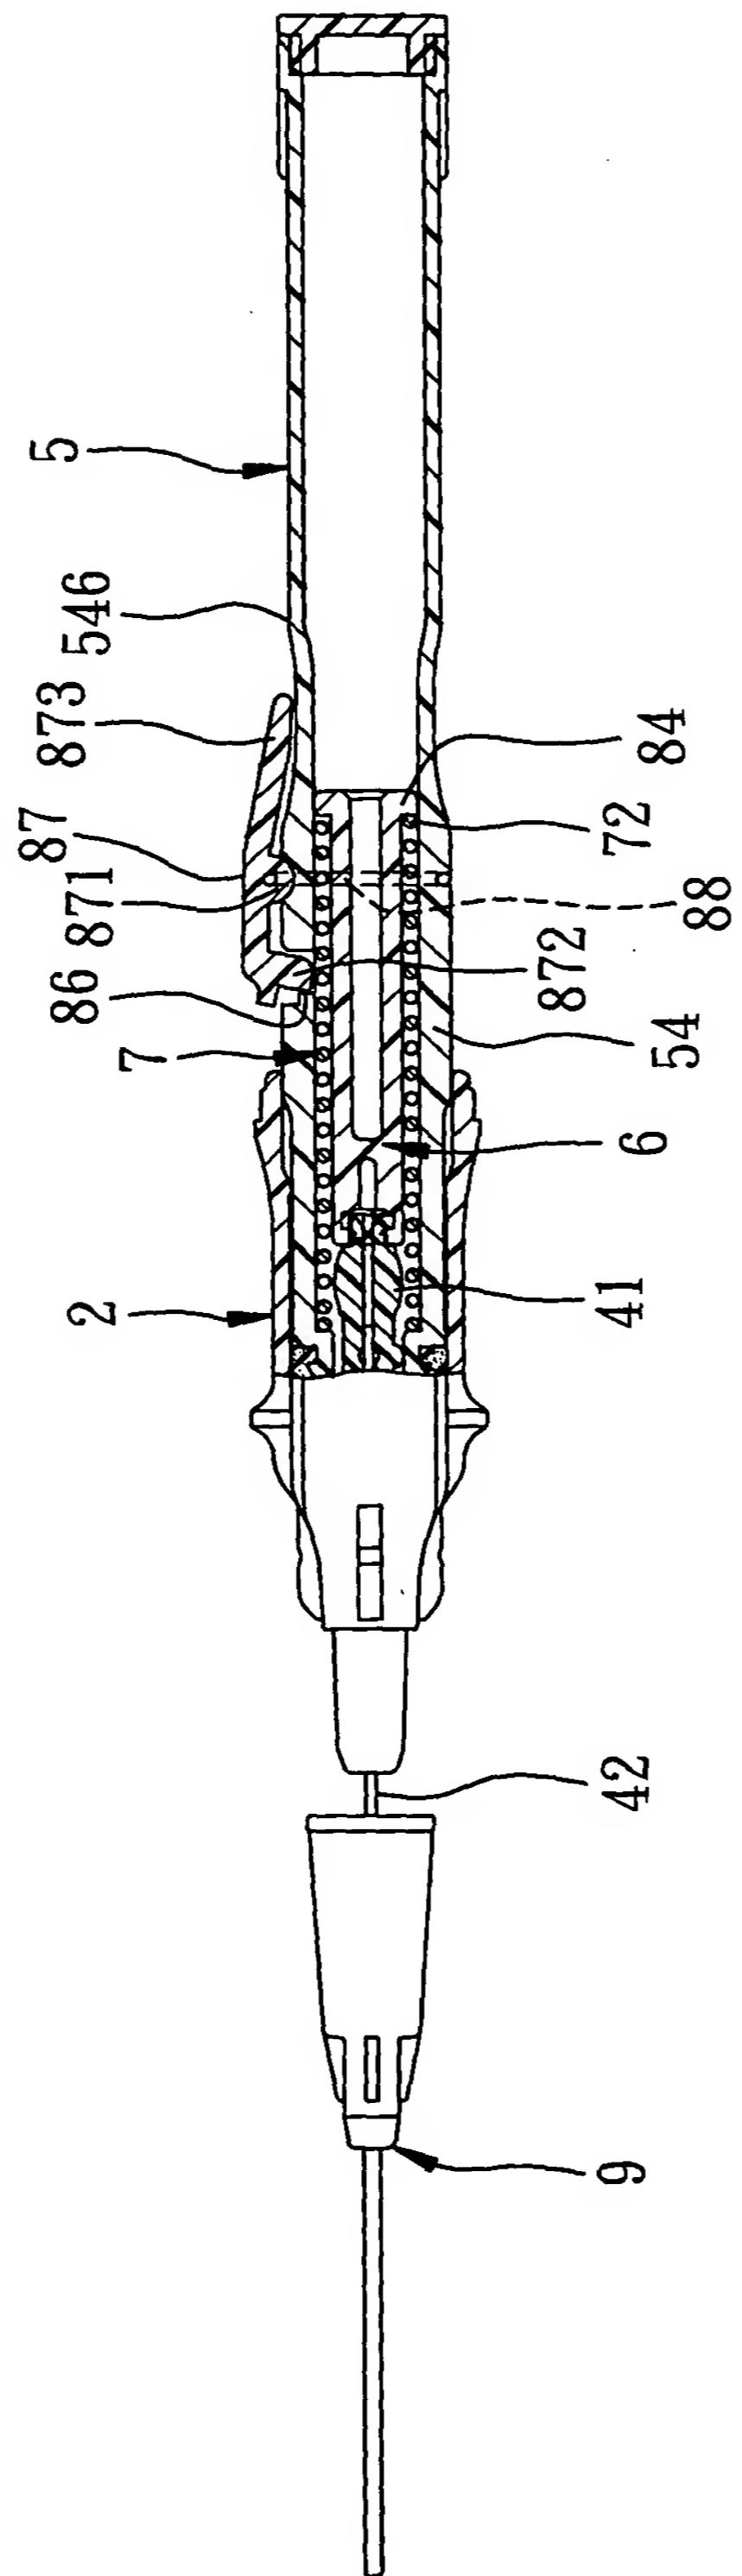


FIG. 26

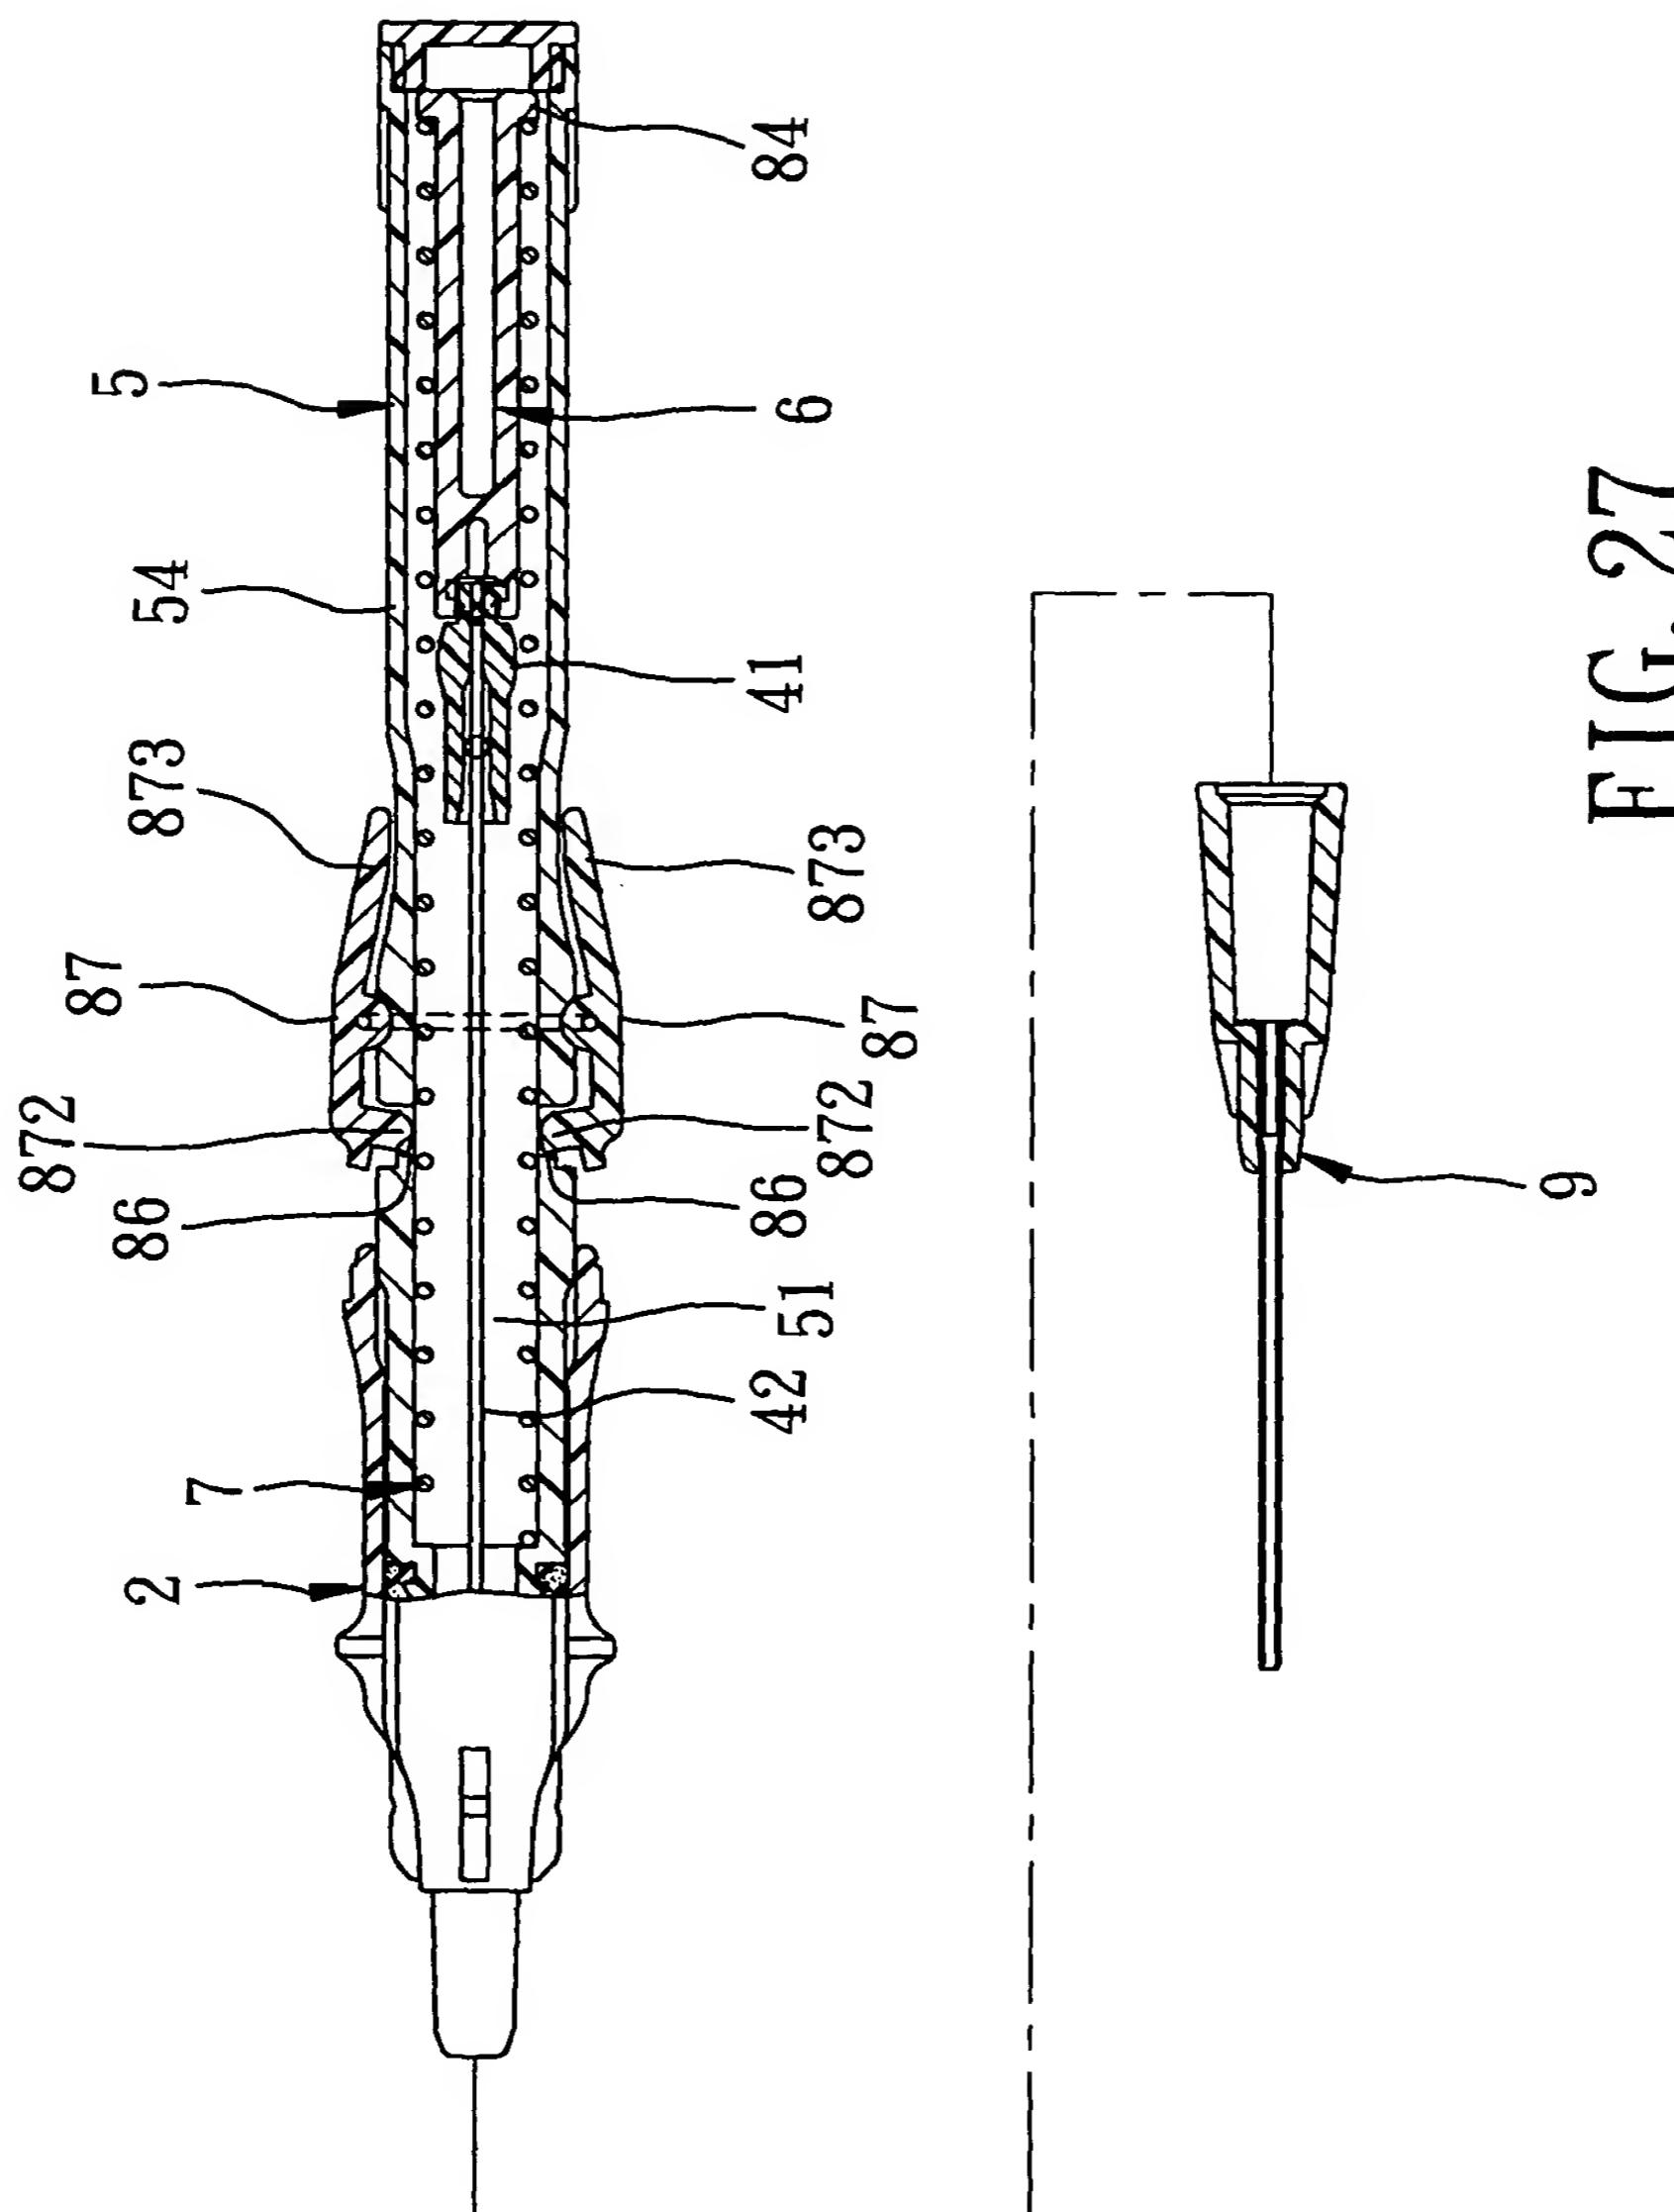


FIG. 27